

iRES⁺

complete
solutions
for oral
surgery




IMPLANT SYSTEMS

PROSTHETIC PARTS

TRADITIONAL AND GUIDED **SURGERY**

IMPLANT CATALOG 2024

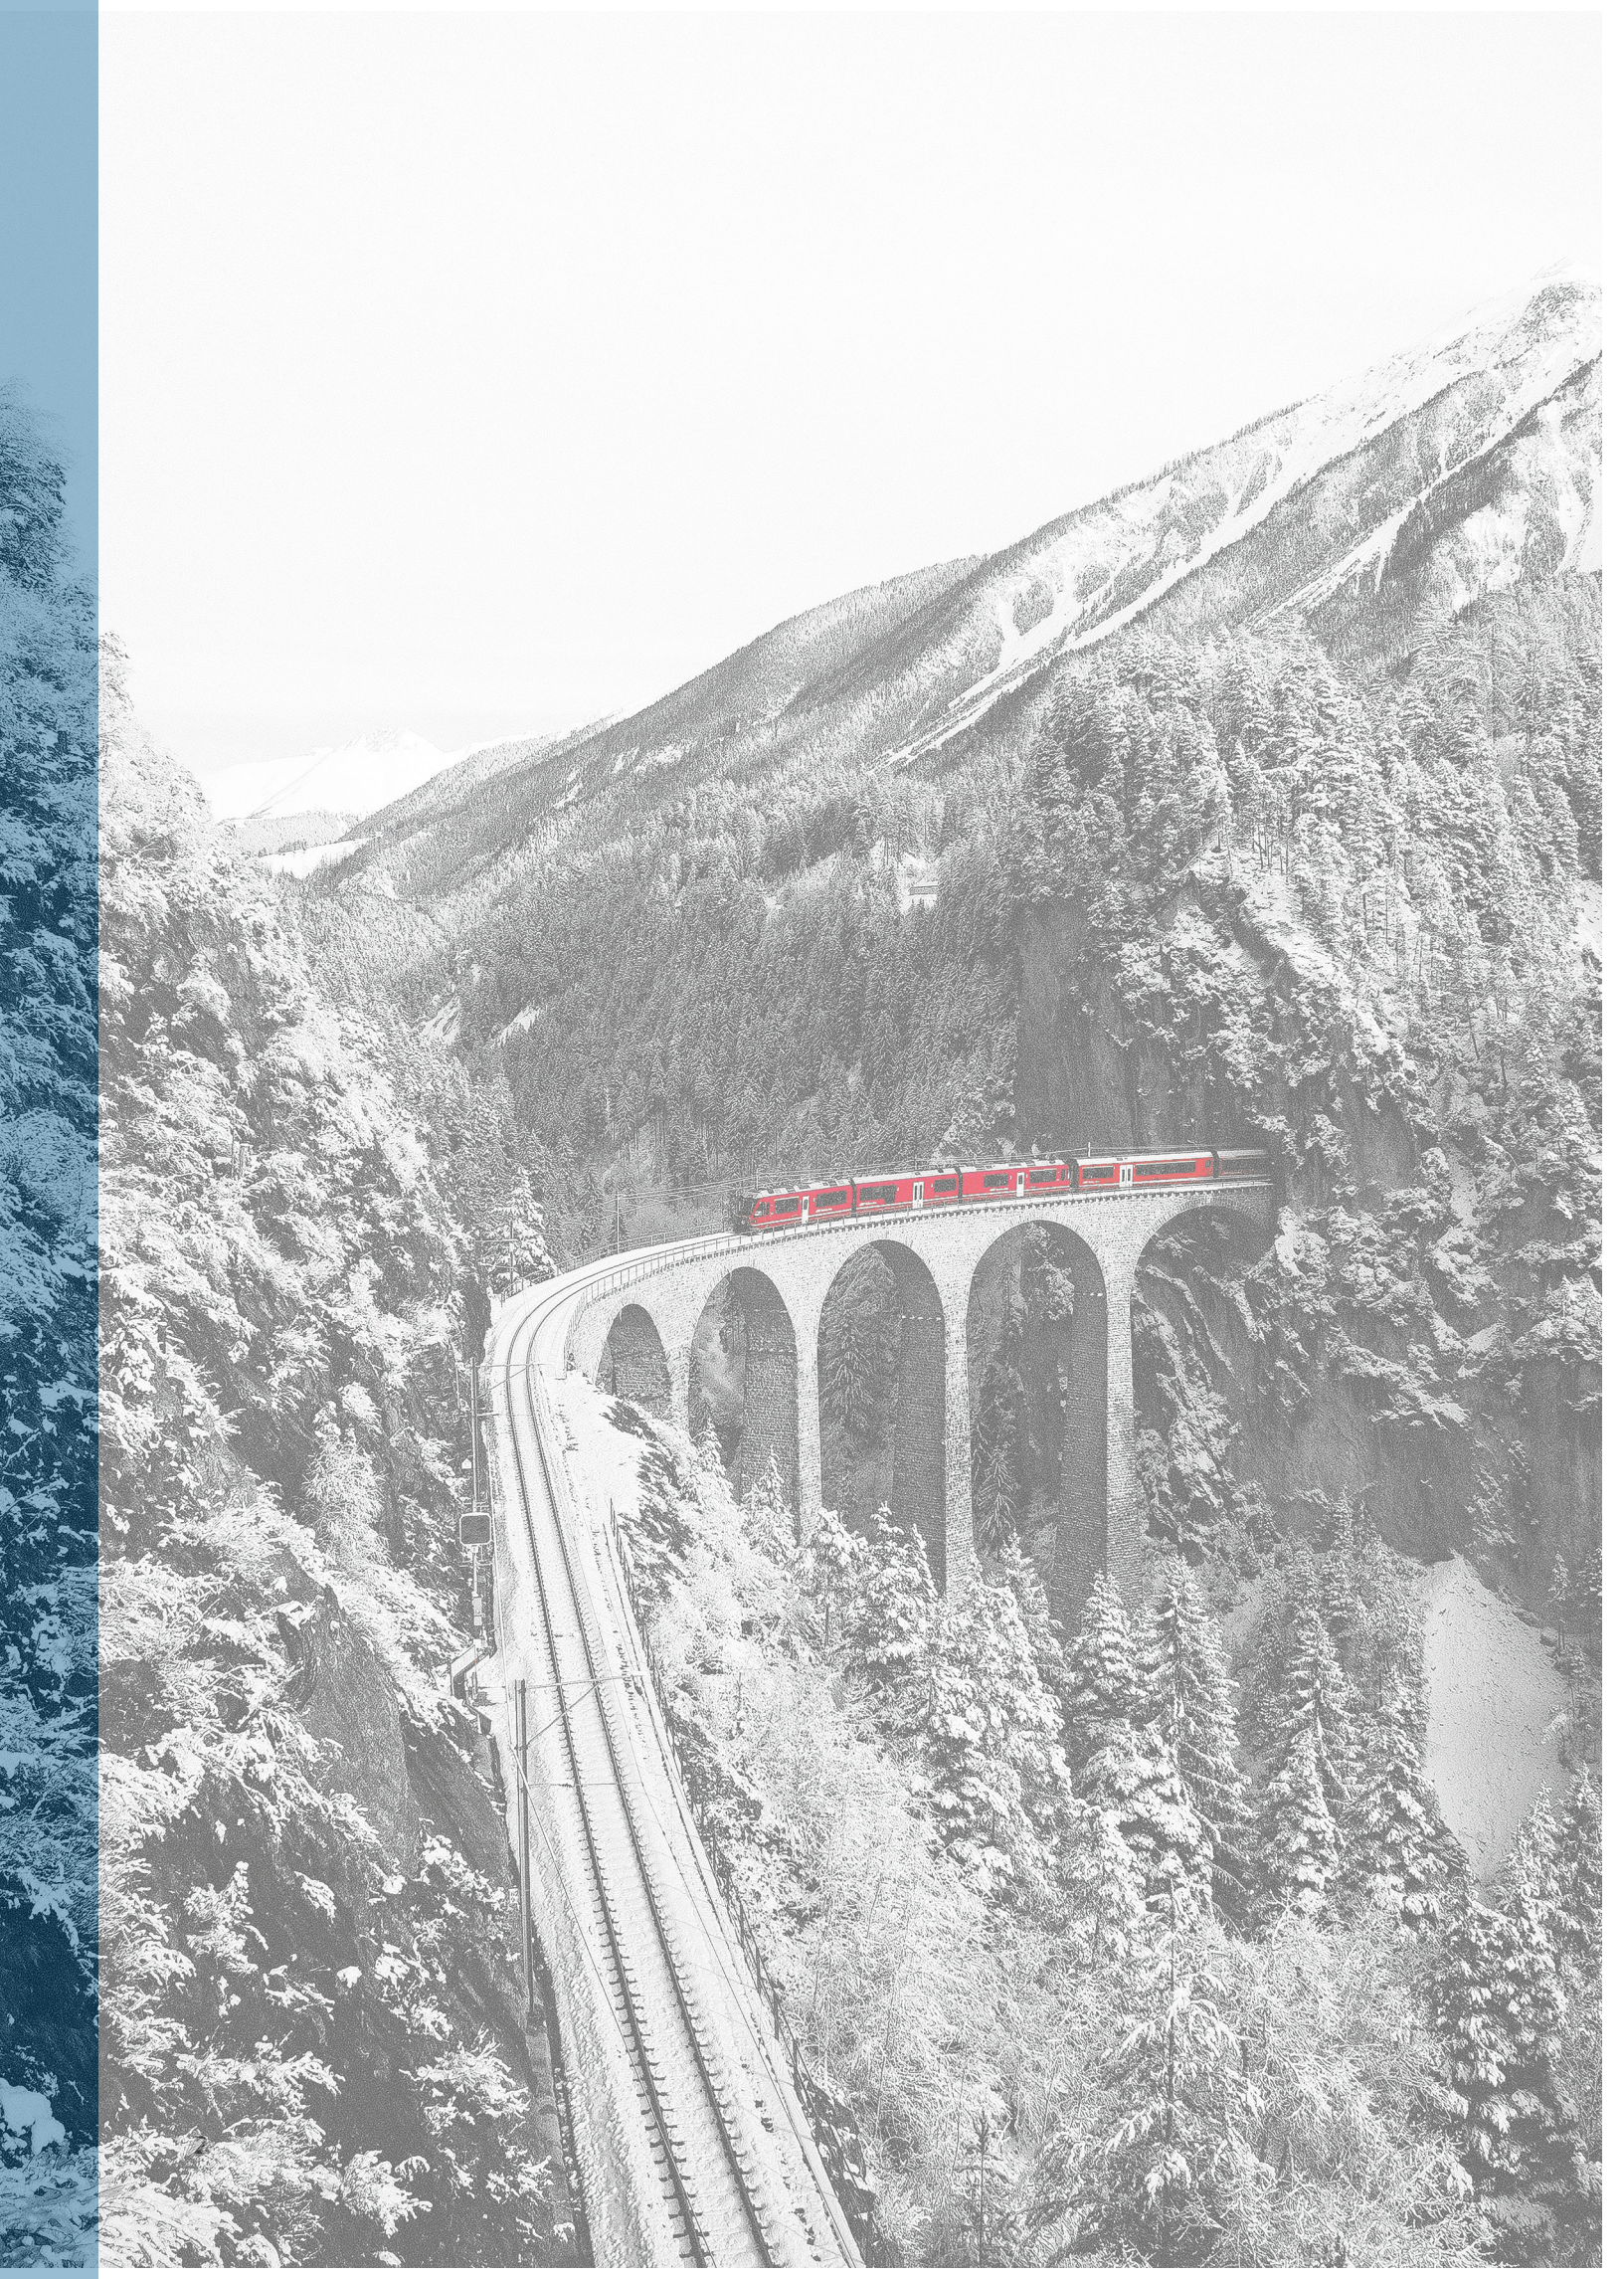



international
Reliable
Efficient
Safe


Reliable results and a short time frame: these indispensable elements of modern oral surgery have been the aim of iRES from the very beginning. This can be observed also in implant lines, designed to offer **maximum simplicity and versatility**.

Thanks to the synergy with top-level **opinion leaders**, such as Prof. Massimo Simion, iRES is one of the first companies to develop **hybrid surface implants**, an additional option that clinicians can adopt for periodontal patients.

INDEX


Bone Level implants	p. 05
iMAX ø 3.3 internal hexagon 2.1	p. 06
Volution ø 3.3 internal hexagon 2.1	p. 07
Prosthetic components iMAX - Volution ø 3.3 internal hexagon 2.1	p. 08
Shapeone ø 3.7 - 4.1 - 4.7 internal hexagon 2.5	p. 13
iMAX ø 3.7 - 4.1 - 4.7 - 5.2 internal hexagon 2.5	p. 14
Volution ø 3.7 - 4.1 - 4.7 - 5.2 internal hexagon 2.5	p. 15
Prosthetic components Shapeone - iMAX - Volution ø 3.7 - 4.1 - 4.7 - 5.2 internal hexagon 2.5	p. 16
iMAX ø 3.3 external hexagon 2.4	p. 22
Prosthetic components iMAX ø 3.3 external hexagon 2.4	p. 23
iMAX ø 3.7 - 4.1 - 4.7 - 5.2 external hexagon 2.7	p. 27
Prosthetic components iMAX ø 3.7 - 4.1 - 4.7 - 5.2 external hexagon 2.7	p. 28
iMAX NHSIC ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2 conometric connection 2.1	p. 32
Prosthetic components iMAX NHSIC ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2 conometric connection 2.1	p. 33
iRETOR accessories	p. 37
MUA components	p. 38
Tissue Level implants	p. 40
Shapeone ø 3.7 - 4.1 - 4.7 internal octagon 3.1	p. 41
Prosthetic components Shapeone ø 3.7 - 4.1 - 4.7 internal octagon 3.1	p. 42
Shapeone ø 3.7 - 4.1 - 4.7 internal hexagon 2.5	p. 44
Prosthetic components Shapeone ø 3.7 - 4.1 - 4.7 internal hexagon 2.5	p. 45
iMAX mua ø 3.3 - 3.7 - 4.1 one piece platform 4.3	p. 46
Prosthetic components iMAX mua ø 3.3 - 3.7 - 4.1 one piece platform 4.3	p. 47
Shapemini implants ball attachment in TIN ø 2.7 and prosthetic components	p. 49
Implant system - Surface treatment	p. 50
Toxicity test - Decontamination - Sterilization and packaging	p. 51
Surgical kit	p. 52
Prosthetic kit	p. 54
Drills	p. 55
Countersink	p. 56
Taps	p. 57
Connectors	p. 58
Accessories and keys	p. 59
Sinus lift kit	p. 62
Surgical protocol	p. 63
Guided surgery	p. 72
Minimum implant dimensions	p. 78
Instruction leaflets	p. 79

BONE LEVEL IMPIANTS

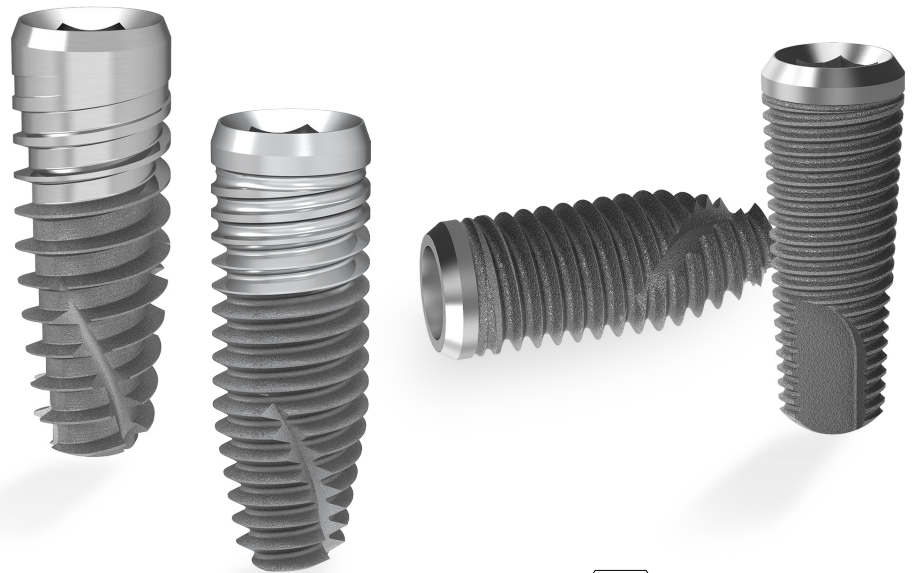


iMAX

INTERNAL HEX \varnothing 3.3 - 3.7 - 4.1 - 4.7 - 5.2



VOLUTION

INTERNAL HEX \varnothing 3.3 - 3.7 - 4.1 - 4.7 - 5.2




SHAPEONE

INTERNAL HEX \varnothing 3.7 - 4.1 - 4.7




iMAX

EXTERNAL HEX \varnothing 3.3 - 3.7 - 4.1 - 4.7 - 5.2



iMAX *NHSIC*



CONO-MORSE NARROW \varnothing 3.3 - 3.7 - 4.1 - 4.7 - 5.2



Dental implants are made of titanium for medical use in compliance with current regulations.



UNIVERSAL SYSTEM
FOR ALL TYPES OF BONES

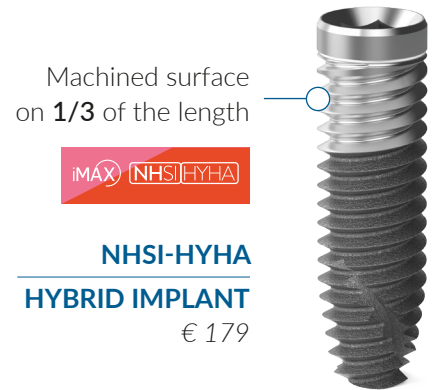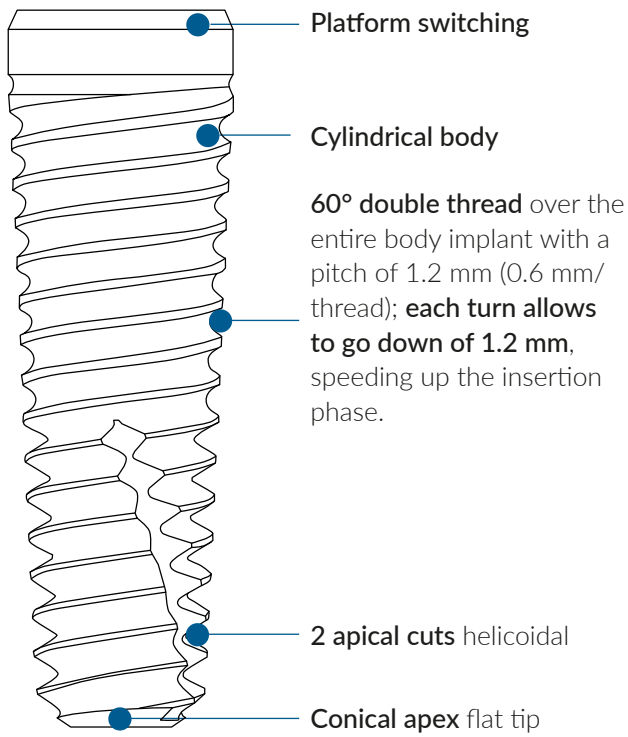

Ø	heights (mm)				implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3,3	10	11.5	13	16	fine double thread 0.6	internal hex	3.2	2,1	1/72

DRIVERS


H	code	€
25	HDH21S	47
30	HDH21L	47

Material: Surgical steel



VOLUTION

LARGE THREAD IMPLANT FOR HIGH PRIMARY STABILITY

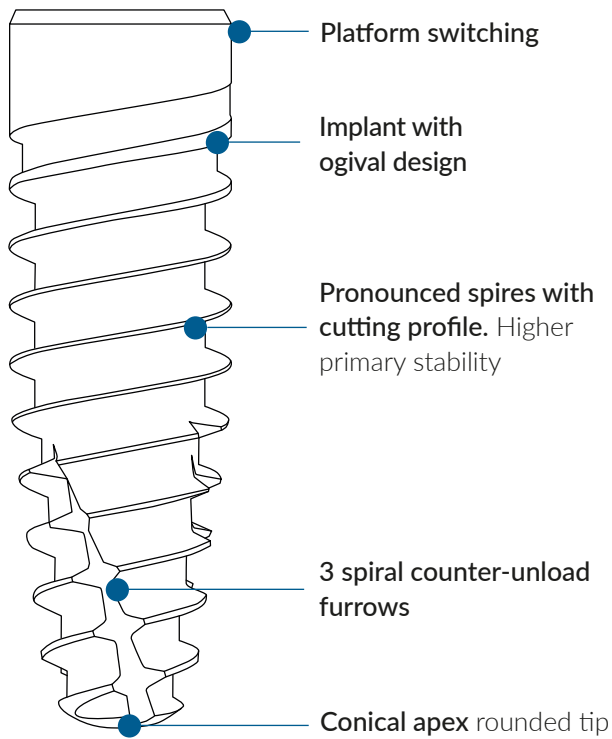

Machined surface on 1/3 of the length



SVB-HYHA
HYBRID IMPLANT

€ 179



1 mm machined neck



SVB-C
NECK MACHINED IMPLANT

€ 147



Full surface treatment



SVB
INTEGRAL IMPLANT

€ 137




Ø	heights (mm)					implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.3	8	10	11.5	13	16	large double thread 0.9	internal hex	3.2	2.1	1/72

CONNECTORS

H	cod.	€
25	HDH21S	47
30	HDH21L	47

Material: Surgical steel




PROSTHETIC COMPONENTS

IMPLANT CONNECTION


Prosthetic components with **Friction Fit** connection have been developed for **SVB** and **NHSI** implant systems with **internal hex** connection.

This connection ensures a **“cold fusion”** between implant and abutment if the retaining screw has been tightened at 30 Ncm. It eliminates micro movements and reduces bacterial infiltration between implant and abutment.

FRICITION FIT
connection with 1° angle
on the abutment

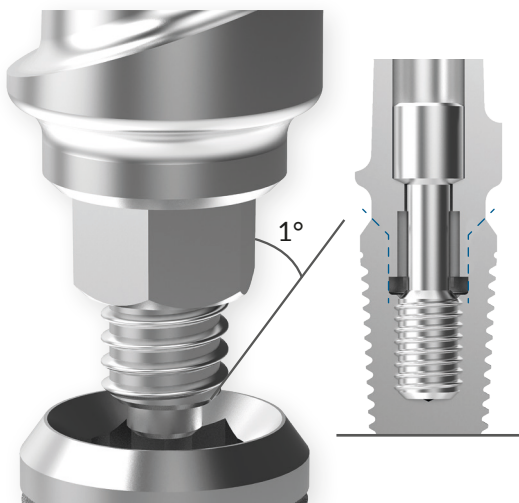

WITHOUT FRICTION FIT
with straight abutment wall

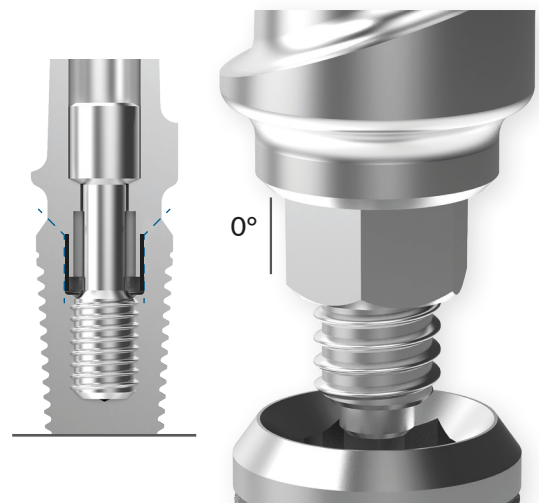

MANAGEMENT OF SOFT TISSUES

The following configurations are available for improved soft tissue management.

STRAIGHT PROFILE



AS



CONCAVE PROFILE




Ø 3.3

SURGICAL SCREWS

Material: Ti-6Al-4V

ø	thread	code	€
3,5	1/72	S1BNCS	16
5	1/72	S1BNCSL	16



Available as spare parts
S1BNCS provided with the implant

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1BRS1	16

For abutments thread 1/72



code	€
S1BRS2	16

For comp MUA thread 1/72



code	€
S1BDTRS	16

Long for transfer thread 1/72



code	€
S1BRS1T6	16

Prosthetic screws torx



HEALING SCREWS

Material: Ti-6Al-4V

ø	H	code	€
3.5	3	S1BN3530HC	26
3.5	4.5	S1BN3545HC	26
3.5	6	S1BN3560HC	26



ø	H	code	€
3.5	1	S1BN3510HCC	26
3.5	3	S1BN3530HCC	26
3.5	4.5	S1BN3545HCC	26
3.5	6	S1BN3560HCC	26



With flared profile

ANALOG

Material: Ti-6Al-4V

code	€
S1BNIA	22



TRANSFER DA IMPRONTA INDIRECTA

Materiale: Ti-6Al-4V

ø	code	€
3,5	S1BN135ITC	68

Screw included: S1BRS1
Indirect transfer cap included



code	€
ITC	21

POM-C indirect transfer cap



ø	code	€
3,5	S1BN1M35	58

Multifunction abutment with flared profile
Screw included: S1BRS1



ø	cod	€
3,5	S1BN1A35	58


Multifunction abutment
Screw included: S1BRS1



DIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1BDTRS

∅	code	€
3.5	S1BNDT35	37




∅	code	€
3.2	S1BN1M35L	58



Multifunction abutment

∅	code	€
5	S1BNDT403	47

3-components for disparallel systems



∅	cod	€
3.5	S1BN1A35L	58

Multifunction abutment



TEMPORARY STRAIGHT ABUTMENTS

Screw included: S1BRS1


∅	code	€
3.5	S1BN135PP	55

Material: PEEK




∅	code	€
3.5	S1BN135P	47

Anti rotation in Ti-6Al-4V



∅	code	€
3.5	S1BN135PR	47

Rotation in Ti-6Al-4V



DEFINITIVE STRAIGHT ABUTMENTS | ANATOMIC

Material: Ti-6Al-4V • Screw included: S1BRS1


∅	code	€
3.5	S1BN135FF	68

Friction Fit




∅	H	code	€
4	1	S1BN1140	58
4	3	S1BN1340	58

Anatomic without Friction Fit



∅	H	code	€
4	1	S1BN1140F	68
4	3	S1BN1340F	68

Anatomic with Friction Fit



code	€
S1BN1TS	58

Abutments for welded technique




DEFINITIVE ANGULATED ABUTMENTS | ANATOMIC

Material: Ti-6Al-4V • Screw included: S1BRS1


∅	H	code	€
4	15° 1	S1BN211540	68
4	15° 3	S1BN231540	68
4	25° 1	S1BN212540	68
4	25° 3	S1BN232540	68

Without Friction Fit



∅	H	code	€
4	15° 1	S1BN211540F	79
4	15° 3	S1BN231540F	79
4	25° 1	S1BN212540F	79
4	25° 3	S1BN232540F	79

Friction Fit



CASTABLE ABUTMENTS

Material: POM-C • Screw included: S1BRS1

∅	code	€
3,5	S1BN3PCR35	30

Rotating



∅	code	€
3,5	S1BN3PC35	30

Non rotating



∅	code	€
3,5	S1BN3PTC45	79

Titanium base: TI-6I-4V



STICKING BASES Digital libraries available

Material: Ti-6Al-4V • Screw included: S1BRS1

∅	code	€
3.5	S1BN135F	68

Friction Fit with emergence profile



∅	code	€
3.5	S1BN135R	58

Rotating with emergence profile



∅	code	€
3.5	S1BN135FS	68

Friction Fit without emergence profile



∅	code	€
3.5	S1BN135RS	58

Rotating without emergence profile



MUA ABUTMENTS Components page 38-39

Material: Ti-6Al-4V

H	code	€
1	S1BN41	58
2	S1BN42	58
3	S1BN43	58
4	S1BN44	58
5	S1BN45	58
6	S1BN46	58



H	code	€
18° 0/2	S1BN518	89
30° 0/2	S1BN532	89

Mounter and S1BRS2 screw included




Tighten with HDH20 driver (page 58)

Mounter included

BALL ABUTMENTS Material: Ti-6Al-4V • CAH and CAT included

∅	H	cod	€
4	1	S1BN61	47
4	2	S1BN62	47
4	3	S1BN63	47
4	4	S1BN64	47
4	5	S1BN65	47



cod	€
CAH	16

Containment ring



cod	€
CALT	8

Nylon containment cap



TIN Treatment on the gold part

Tighten with MDS or MDL screwdriver (page 59)

Ø 3.3

IRETOR *iRETOR accessories page 37*

H	code	€
0	S1BN80	100
1	S1BN81	100
2.5	S1BN825	100
3.5	S1BN835	100
4.5	S1BN845	100
6.5	S1BN865	100



Tighten with 8393 screwdriver (page 60)
 TIN Treatment on the gold part
 Ring and cap not included

COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

code	€
S1BNDIA	22



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1BRS1

	code	€
standard	S1BNSA	58
long	S1BNSAL	58



T-BASE

Material: Ti-6Al-4V • Screw included: S1BRS1 and S1BRS1T6

ø 3,7 shoulder 0,4 cuff	code	€
non rotating	0.8 S1BN11DCTB	79
rotating	0.8 S1BN11DCTBR	79




ø 4,5 shoulder 0,8 cuff	code	€
non rotating	1.8 S1BN12DCTB50	79
rotating	1.8 S1BN12DCTB50R	79



ø 3,7 shoulder 0,4 cuff	code	€
non rotating	1.8 S1BN12DCTB	79
rotating	1.8 S1BN12DCTBR	79



ø 4,5 shoulder 0,8 cuff	code	€
non rotating	2.8 S1BN14DCTB50	79
rotating	2.8 S1BN14DCTB50R	79



ø 3,7 shoulder 0,4 cuff	code	€
non rotating	2.8 S1BN14DCTB	79
rotating	2.8 S1BN14DCTBR	79




Material: Ti-6Al-4V • Screw included: S1BRS1

	code	€
non rotating	S1BN1DTB	68
rotating	S1BN1DTBR	68



CEREC	code	€
non rotating	S1BN1DTBC	68
rotating	S1BN1DTBCR	68




	code	€
On request	S1BRS1T6	16



SHAPEONE

EXCELLENT PRIMARY STABILITY
ALSO IN BONE D4

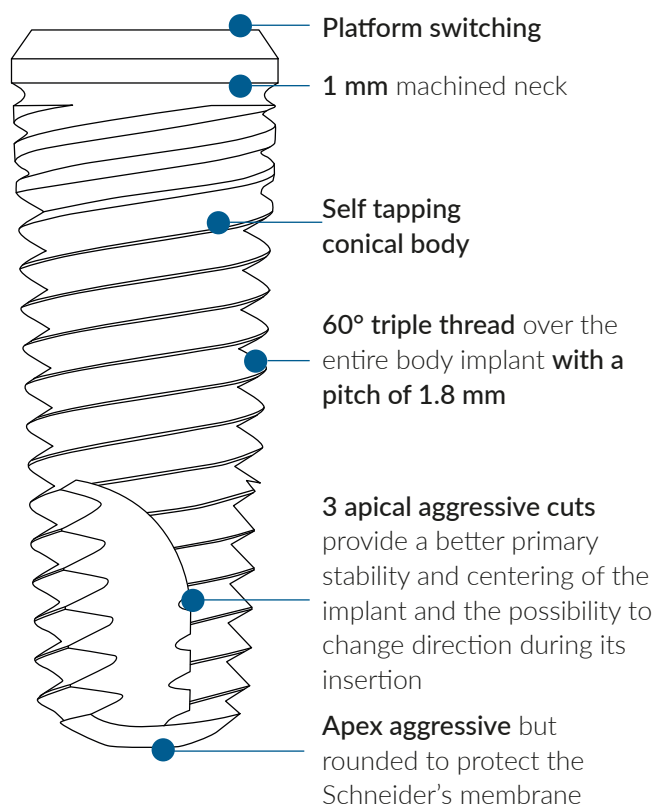

S1B-C
NECK MACHINED
€ 147



Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.7		8	10	11.5	13	16	triple thread 0.6	internal hex	3.5	2.5	1/72
4.1	6.5	8	10	11.5	13	16					
4.7	6.5	8	10	11.5	13	16					

DRIVERS


H	cod.	€
25	HDH25S	47
30	HDH25L	47

Material: Surgical steel





UNIVERSAL SYSTEM FOR ALL TYPES OF BONES

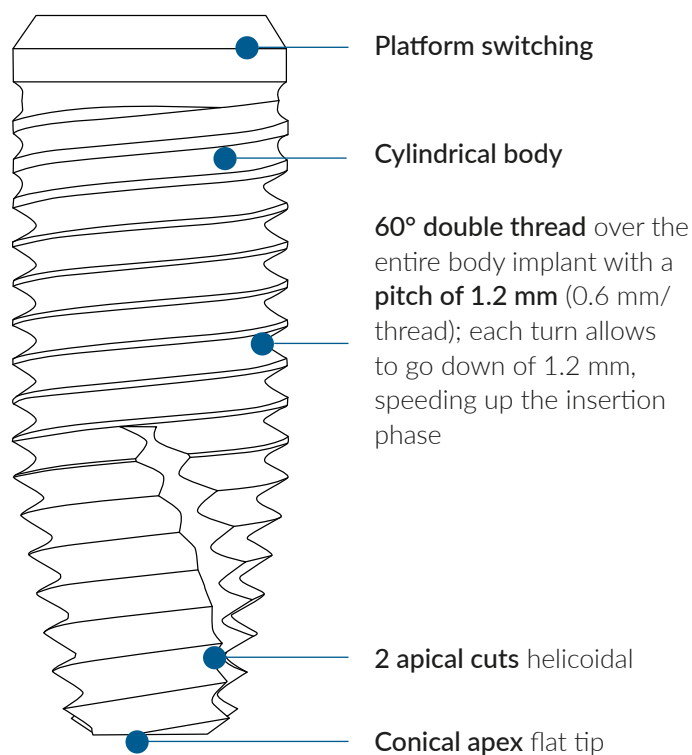

Machined surface on **1/3** of the length



**NHSI-HYHA
HYBRID IMPLANT**

€ 179



1 mm machined neck



**NHSI-C
NECK MACHINED**

€ 147




Ø	heights (mm)					implant thread (mm)	connection	platform (mm)	hex (mm)	thread	
3.7		8	10	11.5	13	16	fine double thread 0.6	internal hex	3.5	2.5	1/72
4.1	6.5	8	10	11.5	13	16					
4.7	6.5	8	10	11.5	13	16					
5.2	6.5	8	10	11.5	13						

DRIVERS


H	cod.	€
25	HDH25S	47
30	HDH25L	47

Material: Surgical steel



VOLUTION

LARGE DOUBLE THREAD IMPLANT FOR BETTER INSERTION FACILITY

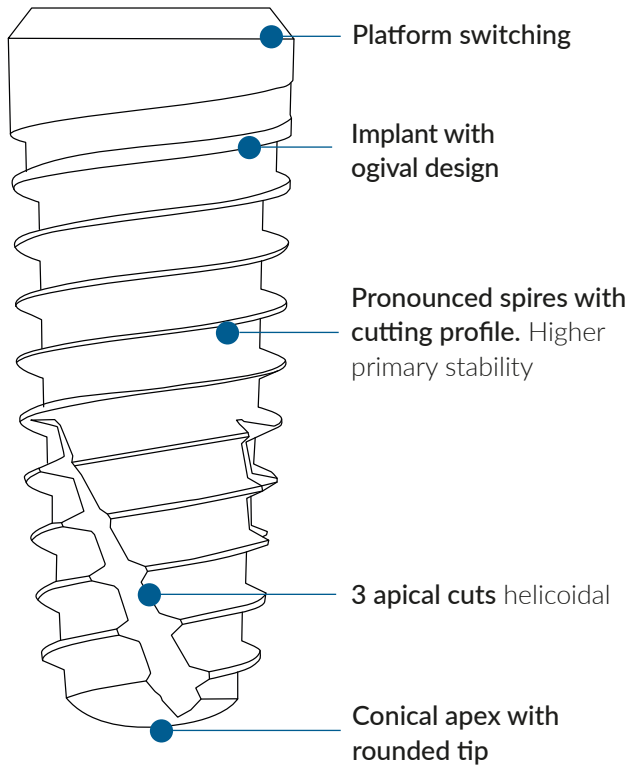

Machined surface on 1/3 of the length



SVB-HYHA
HYBRID IMPLANT

€ 179



1 mm machined neck



SVB-C
NECK MACHINED

€ 147



Full surface treatment



SVB
INTEGRAL IMPLANT

€ 137



Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.7		8	10	11.5	13	16	large double thread 0.9	internal hex	3.5	2.5	1/72
4.1	6.5	8	10	11.5	13	16					
4.7	6.5	8	10	11.5	13	16					
5.2	6.5	8	10	11.5	13						

DRIVERS

H	cod.	€
25	HDH25S	47
30	HDH25L	47

Material: Surgical steel




PROSTHETIC COMPONENTS

IMPLANT CONNECTION


Prosthetic components with **Friction Fit** connection have been developed for **S1B**, **NHSI** and **SVB** implant systems with **internal hex** connection.

This connection ensures a **“cold fusion”** between implant and abutment if the retaining screw has been tightened at 30 Ncm. It eliminates micro movements and reduces bacterial infiltration between implant and abutment.

FRICITION FIT
 connection with 1° angle
 on the abutment

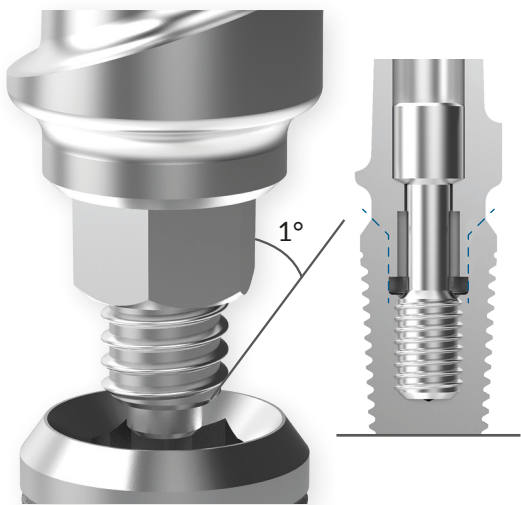

WITHOUT FRICTION FIT
 with straight abutment wall

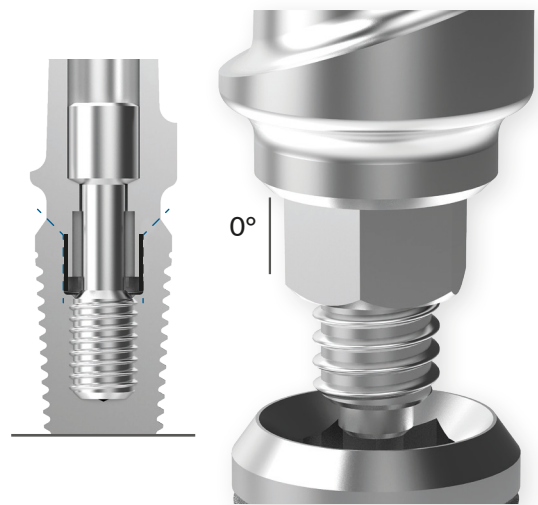

MANAGEMENT OF SOFT TISSUES

The following configurations are available for improved soft tissue management.

STRAIGHT PROFILE



S PROFILE



CONCAVE PROFILE



45° PROFILE



SURGICAL SCREWS

Material: Ti-6Al-4V

Ø	thread	code	€
3.5	1/72	S1BCS	16
5	1/72	S1BCSL	16



Available as spare parts
S1BCS included in the implant

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1BRS1	16

For abutment thread 1/72



code	€
S1BRS2	16

For MUA thread 1/72



code	€
S1BDTRS	16

Long for transfer thread 1/72



code	€
S1BRS1T6	16

Torx screw for digital



HEALING SCREWS

Material: Ti-6Al-4V

Ø	H	code	€
3.5	3	S1B3530HC	26
3.5	4.5	S1B3545HC	26
3.5	6	S1B3560HC	26



Ø	H	code	€
5	3	S1B5030HC	26
5	4.5	S1B5045HC	26
5	6	S1B5060HC	26



Ø	H	code	€
3.5	3	S1B3530HCC	26
3.5	4.5	S1B3545HCC	26
3.5	6	S1B3560HCC	26

Flaring profile



Ø	H	code	€
5	3	S1B5030HCC	26
5	4.5	S1B5045HCC	26
5	6	S1B5060HCC	26

Flaring profile



Ø	H	code	€
6	3	S1B6030HCC	26
6	4.5	S1B6045HCC	26

Flaring profile



ANALOG

Material: Ti-6Al-4V

code	€
S1BIA	22



INDIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1BRS1

∅	code	€
3.5	S1B135ITC	68

Included indirect transfer cap



∅	code	€
5	S1B1A50	58

Multifunction abutment



∅	code	€
5	S1B150ITC	68

Included indirect transfer cap



code	€
ITC	21

Indirect transfer cap
Material: POM-C



DIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V


∅	code	€
3.5	S1BDT35	37

Screw included: S1BDTRS



∅	code	€
5	S1BDT50	37

Screw included: S1BDTRS



∅	code	€
5	S1B1A50L	58

Multifunction abutment
Screw included: S1BDTRS



∅	code	€
5	S1B1M50L	58

Multifunction abutment with flared profile
Screw included: S1BDTRS and S1BRS1



∅	code	€
5	S1BDT503	47

3-components for disparallel systems



TEMPORARY STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1BRS1

∅	code	€
4	S1B140P	47

Not rotating



∅	code	€
4	S1B140PR	47

Rotating



Material: PEEK • Screw included: S1BRS1

∅	code	€
4	S1B140PP	58



DEFINITIVE STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1BRS1

Ø	code	€
3.5	S1B135F	68
5	S1B150F	68



Friction Fit

Ø	H	code	€
4.5	1	S1B1145	58
4.5	3	S1B1345	58



Anatomic without Friction Fit

code	€
S1B1TS	58



Rotating abutment for welded technique

Ø	code	€
4.5	S1B145FS	68
5.5	S1B155FS	68



Friction Fit without emergence profile

Ø	H	code	€
4.5	1	S1B1145F	68
4.5	3	S1B1345F	68



Anatomic with Friction Fit

ANGLED ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1BRS1

Ø	code	€
4.5	S1B250F	79



Friction Fit

Ø	code	€
4.5	S1B245FS	79




Friction Fit without emergence

ANATOMIC DEFINITIVE ANGLED ABUTMENTS


Material: Ti-6Al-4V • Screw included: S1BRS1

Ø	H	code	€	
4.5	15°	1	S1B211545	68
4.5	15°	3	S1B231545	68
4.5	25°	1	S1B212545	68
4.5	25°	3	S1B232545	68



Without Friction Fit

Ø	H	code	€	
4.5	15°	1	S1B211545F	79
4.5	15°	3	S1B231545F	79
4.5	25°	1	S1B212545F	79
4.5	25°	3	S1B232545F	79



Friction Fit

CASTABLE ABUTMENTS

Material: POM-C • Screw included: S1BRS1

Ø	code	€
4.5	S1B3PC45	30



Not rotating

Ø	code	€
4.5	S1B3PCR45	30



Rotating

code	€
S1B3PTC45	79



Titanium base: TI-6Al-4V

STICKING BASES Digital libraries available

Material: Ti-6Al-4V • Screw included: S1BRS1

ø	code	€
4,5	S1B140F	68

Friction Fit with emergence profile



ø	code	€
4,5	S1B140R	58

Rotating with emergence profile



ø	code	€
3,5	S1B140FS	68

Friction Fit without emergence profile



ø	code	€
4,5	S1B140RS	58

Rotating without emergence profile



MUA BUTMENTS Components page 38-39

Material: Ti-6Al-4V

H	code	€
1	S1B41	58
2	S1B42	58
3	S1B43	58
4	S1B44	58
5	S1B45	58
6	S1B46	58



H	code	€
18° 0/2	S1B518	89
30° 0/2	S1B532	89
30° 2/4	S1B534	89



Mounter and S1BRS2 screw included
Tighten with HDH20 driver (page 58)

Mounter included
Tighten with HDH20 driver (page 58)

BALL BUTMENTS Material: Ti-6Al-4V • CAH and CAT included

H	code	€
1	S1B61	47
2	S1B62	47
3	S1B63	47
4	S1B64	47
5	S1B65	47



code	€
CAH	16

Containment ring



code	€
CALT	8

Nylon containment cap



TIN Treatment on the gold part
Tighten with MDS or MDL screwdriver (page 59)

IRETOR iRETOR accessories page 37

H	code	€
0	S1B80	100
1	S1B81	100
2.5	S1B825	100
3.5	S1B835	100
4.5	S1B845	100
6.5	S1B865	100



Tighten with 8393 screwdriver (page 60)
TIN Treatment on the gold part
Ring and cap not included

COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

code	€
S1BDIA	22



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1BRS1

	code	€
standard	S1BSA	58
long	S1BSAL	58



T-BASE

Material: Ti-6Al-4V • Screw included: S1BRS1 and S1BRS1T6

ø 3.4 shoulder 0.4 cuff	code	€
not rotating 0	S1B00DCTB	79
rotating 0	S1B00DCTBR	79



ø 4.5 shoulder 0.8 cuff	code	€
not rotating 1.8	S1B12DCTB50	79
rotating 1.8	S1B12DCTBR50	79



ø 3.7 shoulder 0.4 cuff	cod	€
not rotating 0.4	S1B11DCTB	79
rotating 0.4	S1B11DCTBR	79
not rotating 1.8	S1B12DCTB	79
rotating 1.8	S1B12DCTBR	79



ø 5.7 shoulder 1.2 cuff	code	€
not rotating 1.8	S1B14DCTBR	79
rotating 1.8	S1B14DCTB	79
not rotating 2.8	S1B14DCTB50	79
rotating 2.8	S1B14DCTBR50	79



Material: Ti-6Al-4V • Screw included: S1BRS1

ø 3,7 spalla 0,5 cuff	code	€
not rotating 0.2	S1B1DTB	68
rotating 0.2	S1B1DTBR	68



CEREC	code	€
not rotating	S1B1DTBC	68
rotating	S1B1DTBCR	68




	code	€
On request	S1BRS1T6	16



iMAX

UNIVERSAL SYSTEM FOR ALL TYPES OF BONES

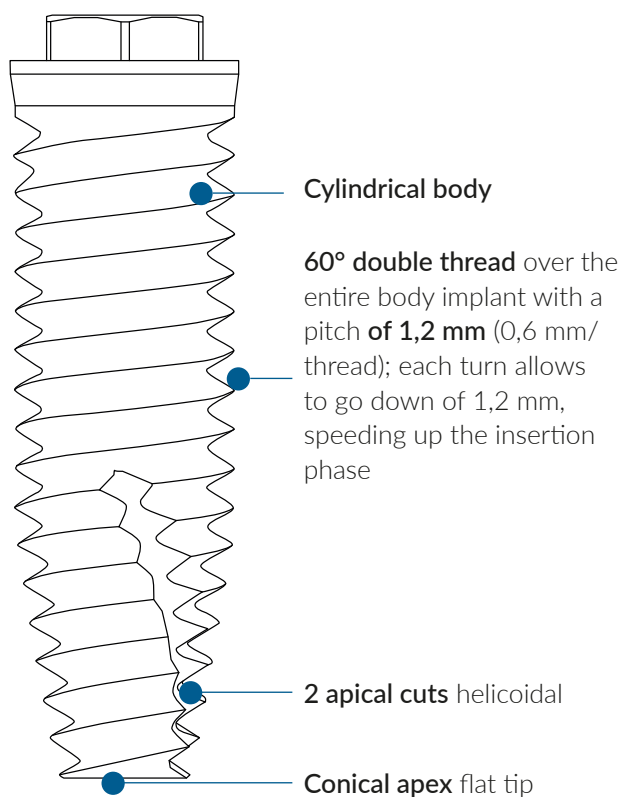

Machined surface on **1/3** of the length




NHSE-HYHA
HYBRID IMPLANT
€ 179



1 mm machined neck



NHSE-C
NECK MACHINED
€ 147



Ø	heights (mm)				implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.3	10	11.5	13	16	fine double thread 0.6	external hex	3.5	2.4	1.6

DRIVERS

H	code	€
25	HDH24S	47
30	HDH24L	47


Material: Surgical steel



PROSTHETIC COMPONENTS

IMPLANT CONNECTION

A “flat to flat” connection for external hex is especially suitable for NHSE implant systems.

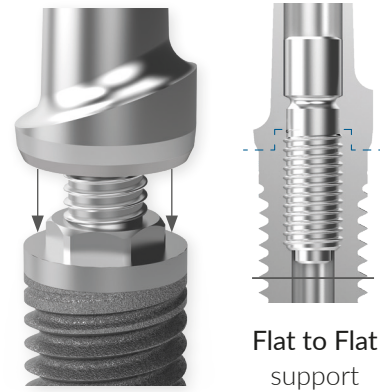

Flat to Flat support

SURGICAL SCREWS

Material: Ti-6Al-4V

ø	thread	code	€
3.5	1.6	S1EHNCS	16



Provided with the implant
Available as spare parts

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1EHNRS1	16



For abutment thread 1.6 mm

code	€
S1EHNRS2	16



For abutment thread 1.6 mm

code	€
S1EHNDRS	16



Long for transfer thread 1.6 mm

code	€
S1EHNRS1T6	16



Torx screw for digital

HEALING SCREWS

Material: Ti-6Al-4V

ø	H	code	€
3.5	3	S1EHN3530HC	26
3.5	4.5	S1EHN3545HC	26
3.5	6	S1EHN3560HC	26



ANALOGO

Material: Ti-6Al-4V

code	€
S1EHNIA	22



DIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1EHNDRS

∅	cod	€
3.5	S1EHNDR35	37



∅	cod	€
3.2	S1EHN1A35L	68



Multifunction

TEMPORARY STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1EHNRS1

∅	cod	€
3.5	S1EHN135P	47



Not rotating

∅	cod	€
3.5	S1EHN135PR	47



Rotating

DEFINITIVE STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1EHNRS1

∅	cod	€
3.5	S1EHN1A35	68



Multifunction

∅	cod	€
4	S1EHN140	68



Not rotating

∅	H	cod	€
4	1	S1EHN1135	68
4	3	S1EHN1335	68



Anatomic

cod	€
S1EHN1TS	58



Abutments for welded technique

STICKING BASES

Material: Ti-6Al-4V • Screw included: S1EHNRS1

∅	cod	€
4	S1EHN135	68



Not rotating

∅	cod	€
4	S1EHN135R	58




Rotating

DEFINITIVE ANGLED ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1EHNRS2

∅	H	cod	€
4	15° 1	S1EHN211540	79
4	15° 3	S1EHN231540	79
4	25° 1	S1EHN212540	79
4	25° 3	S1EHN232540	79



CASTABLE ABUTMENTS

Material: POM-C • Screw included: S1EHNRS1

∅	cod	€
3.5	S1EHN3PC35	30

Not rotating



∅	cod	€
4	S1EHN3PCR35	30


Rotating




MUA ABUTMENTS Components page 38-39

Material: Ti-6Al-4V

∅	H	cod	€
3.5	1	S1EHN41	58
3.5	2	S1EHN42	58
3.5	3	S1EHN43	58
3.5	4	S1EHN44	58
3.5	5	S1EHN45	58



∅	H	cod	€
3.5	18° 0/2	S1EHN518	89
3.5	30° 0/2	S1EHN532	89




Mounter and S1EHNRS2 screw included

Mounter included

Tighten with HDH20 driver (page 58)

BALL ABUTMENTS Material: Ti-6Al-4V • CAH and CALT included

∅	H	cod	€
3.5	1	S1EHN61	47
3.5	2	S1EHN62	47
3.5	3	S1EHN63	47
3.5	4	S1EHN64	47



cod	€
CAH	16

Containment ring



cod	€
CALT	8

Nylon containment cap




TIN Treatment on the gold part

Tighten with MDS or MDL screwdriver (page 59)

IRETOR iRETOR accessories page 37

H	cod	€
0	S1EHN80	100
1	S1EHN81	100
2.5	S1EHN825	100
3.5	S1EHN835	100
4.5	S1EHN845	100
6.5	S1EHN865	100



Tighten with 8393 screwdriver (page 60)

TIN Treatment on the gold part

Ring and cap not included

COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://it.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

cod	€
S1EHNDIA	22



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1EHNRS1

cod	€
S1EHNSA	58



T-BASE

Material: Ti-6Al-4V • Screw included: S1EHNRS1

	cod	€
non rotating	S1EHN1DTB	74
rotating	S1EHN1DTBR	74




	cod	€
On request	S1EHNRS1T6	16



Colored internal prosthetic part



UNIVERSAL SYSTEM
FOR ALL TYPES OF BONES

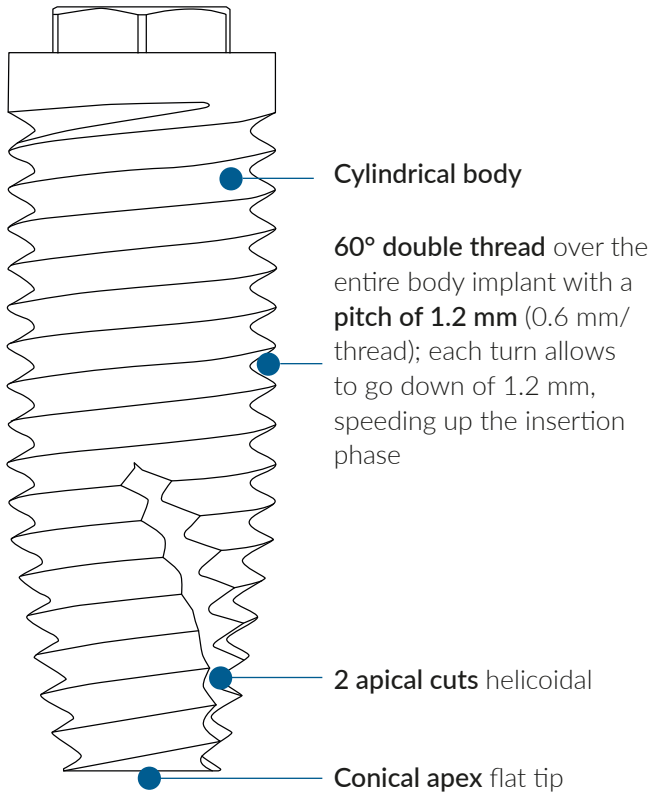

Machined surface on 1/3 of the length



NHSE-HYHA
IBRID IMPLANT
€ 179



1 mm machined neck



NHSE-C
NECK MACHINED
€ 147



Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.7	6.5	8	10	11.5	13	16	fine double thread 0.6	external hex	4.1	2.7	2.0
4.1	6.5	8	10	11.5	13	16					
4.7	6.5	8	10	11.5	13	16					
5.2	6.5	8	10	11.5	13	16					

DRIVERS

H	cod.	€
25	HDH27S	47
30	HDH27L	47


Material: Surgical steel



PROSTHETIC COMPONENTS

IMPLANT CONNECTION

A "flat to flat" connection for external hex is especially suitable for NHSE implant systems.

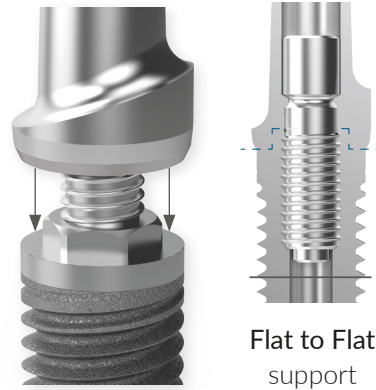

SURGICAL SCREWS

Material: Ti-6Al-4V

ø	thread	code	€
4.1	2	S1EHCS	16



Provided with the implant
Available as spare parts

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1EHRS1	16



For abutment thread 2 mm

code	€
S1EHRS2	16



For abutment thread 2 mm

code	€
S1EHDTRS	16



Long for transfer thread 2 mm

code	€
S1EHRS1T6	16



Torx screw for prosthesis

HEALING SCREWS

Material: Ti-6Al-4V

ø	H	code	€
4.1	3	S1EH4130HC	26
4.1	5	S1EH4145HC	26
4.1	6	S1EH4160HC	26



ø	H	code	€
5	3	S1EH5030HC	26
5	5	S1EH5045HC	26
5	6	S1EH5060HC	26



ANALOG

Material: Ti-6Al-4V

code	€
S1EHIA	22



DIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1EHDTRS

∅	cod	€
4.1	S1EHDT41	37
5	S1EHDT50	37



∅	cod	€
5	S1EH1A50L	58



Multifunction

MONCONI PROVVISORI

Material: Ti-6Al-4V • Screw included: S1EHR1

∅	cod	€
4.1	S1EH141P	47

Not rotating



∅	cod	€
4.1	S1EH141PR	47

Rotating



DEFINITIVE STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1EHR1

∅	cod	€
5	S1EH1A50	68

Multifunction



∅	cod	€
5	S1EH150	68

Not rotating



∅	H	cod	€
4.1	1	S1EH1141	68
4.1	3	S1EH1341	68

Anatomic



∅	cod	€
5	S1EH1TS	58

Abutments for welded technique



STICKING BASES

Material: Ti-6Al-4V • Screw included: S1EHR1

∅	cod	€
4.1	S1EH141	68

Not rotating



∅	cod	€
4.1	S1EH141R	58


Rotating



DEFINITIVE ANGLED ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1EHR2

∅	H	cod	€
4	15° 1	S1EH211550	79
4	15° 3	S1EH231550	79
4	25° 1	S1EH212550	79
4	25° 3	S1EH232550	79



CASTABLE ABUTMENTS

Material: POM-C • Screw included: S1EHR51

ø	code	€
4,1	S1EH3PC41	30



ø	cod	€
4,1	S1EH3PCR41	30

Rotating



MUA ABUTMENTS Components page 38-39

Material: Ti-6Al-4V

ø	H	code	€
4,1	1	S1EH41	58
4,1	2	S1EH42	58
4,1	3	S1EH43	58
4,1	4	S1EH44	58
4,1	5	S1EH45	58



ø	H	code	€
4,1	18° 0/2	S1EH518	89
4,1	30° 0/2	S1EH532	89
4,1	30° 2/4	S1EH534	89




Mounter and S1EHR52 screw included

Tighten with HDH20 driver (page 58)
Mounter included

BALL ABUTMENTS Material: Ti-6Al-4V • CAH and CAT included

ø	H	code	€
4,1	1	S1EH61	47
4,1	2	S1EH62	47
4,1	3	S1EH63	47
4,1	4	S1EH64	47



code	€
CAH	16

Containment ring



code	€
CALT	8

Nylon containment cap



TIN Treatment on the gold part
Tighten with MDS or MDL screwdriver (page 59)

IRETOR iRETOR accessories page 37

H	code	€
0	S1EH80	100
1	S1EH81	100
2,5	S1EH825	100
3,5	S1EH835	100
4,5	S1EH845	100
6,5	S1EH865	100



Tighten with 8393 screwdriver (page 60)
TIN Treatment on the gold part
Ring and cap not included

Ø 3.7 - 4.1 - 4.7 - 5.2

COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V


code	€
S1EHDIA	22



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1EHR1

code	€
S1EHS1	58



T-BASE

Material: Ti-6Al-4V • Screw included: S1EHR1

	code	€
Not rotating	S1EH1DTB	74
Rotating	S1EH1DTBR	74




	code	€
On request	S1EHR1T6	16



Colored internal prosthetic part

iMAX NHSIC

UNIVERSAL SYSTEM FOR ALL TYPES OF BONES

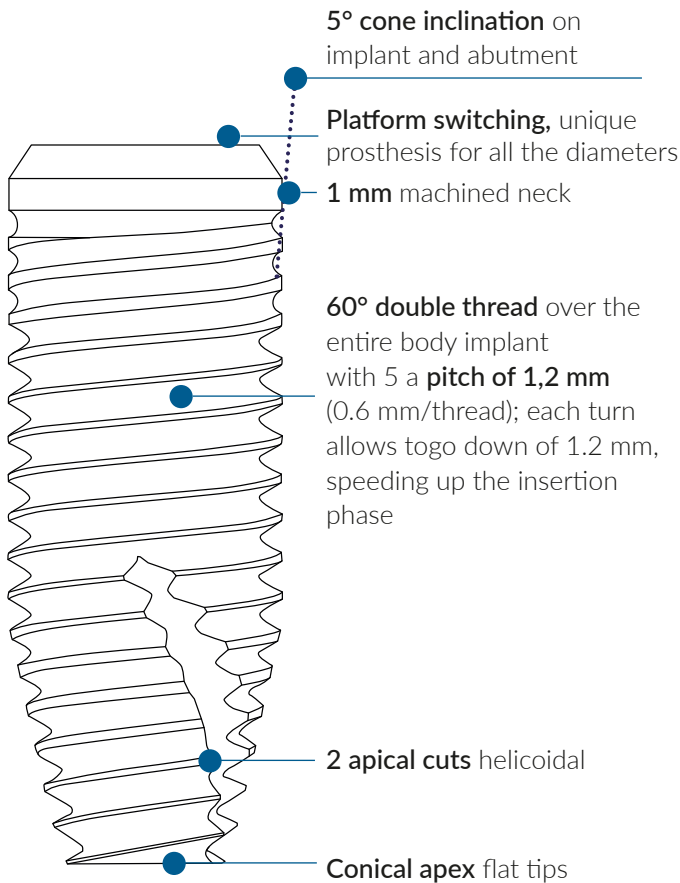

NHSIC-C
NECK MACHINED
€ 163



CONO-MORSE NARROW 2.1 | BONE LEVEL | Ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2

Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	hex (mm)	thread
3.3			10	11.5	13	16	fine double thread 0.6	cono-morse	narrow	2,1	1/72
3.7		8	10	11.5	13	16					
4.1	6.5	8	10	11.5	13	16					
4.7	6.5	8	10	11.5	13	16					
5.2	6.5	8	10	11.5	13						

DRIVERS

H	cod.	€
25	HDH21S	47
30	HDH21L	47





Material: Surgical steel

PROSTHETIC COMPONENTS

IMPLANT CONNECTION

The **NHSIC** conical connection has a **5° angle** on the abutment and on the implant, and an emergence profile for the mucous attack. The **cone-morse** connection creates fissures (1µm) smaller than bacteria, absorbs vibration and chewing stress with the result that it eliminates the unscrewing of the screws.

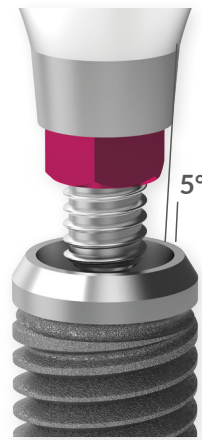

CONOMETRICS
5° angle on the implant and on the abutment

MANAGEMENT OF SOFT TISSUES

The following configurations are available for improved soft tissue management.

CONCAVE PROFILE



SURGICAL SCREWS

Material: Ti-6Al-4V

code	€
NHSICNCS	16



Provided with the implant
Available as spare parts

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1BRS1	16

For abutment thread 1/72



code	€
S1BRS2	16

For MUA thread 1/72



code	€
S1BDTRS	16

Long for transfer thread 1/72



code	€
S1BRS1T6	16

Torx screw for prosthesis



Ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2

HEALING SCREWS

Material: Ti-6Al-4V • Screw included: S1BRS1

ø	H	cod	€
4	3	NHSICN4030HC	32
4	4,5	NHSICN4045HC	32
4	6	NHSICN4060HC	32



ANALOG

Material: Ti-6Al-4V


ø	cod	€
4	NHSICNIA	27



DIRECT TRANSFER IMPRESSION

Material: Ti-6Al-4V • Screw included: S1BDTRS


ø	H	cod	€
4	1	NHSICNDT140	47
4	2	NHSICNDT240	47
4	4	NHSICNDT440	47



PEEK TEMPORARY ABUTMENTS

Material: PEEK • Screw included: S1BRS1


ø	H	cod	€
4	1	NHSICN1140PP	53
4	2	NHSICN1240PP	53
4	4	NHSICN1440PP	53



STRAIGHT ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1BRS1

ø	H	cod	€
4	1	NHSICN1140	89
4	2	NHSICN1240	89
4	4	NHSICN1440	89




Not rotating

STICKING BASES


Material: Ti-6Al-4V • Screw included: S1BRS1

ø	H	cod	€
4	1	NHSICN1140SB	79
4	2	NHSICN1240SB	79
4	4	NHSICN1440SB	79



Not rotating

ø	H	cod	€
4	1	NHSICN1140RSB	79
4	2	NHSICN1240RSB	79
4	4	NHSICN1440RSB	79




Rotating

Ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2

ANGLED ABUTMENTS

Material: Ti-6Al-4V • Screw included: S1BRS1

Ø	H		cod	€
4	15°	1	NHSICN211540	89
4	15°	2	NHSICN221540	89
4	15°	4	NHSICN241540	89
4	25°	1	NHSICN212540	89
4	25°	2	NHSICN222540	89
4	25°	4	NHSICN242540	89



MUA ABUTMENTS Components page 38-39

Material: Ti-6Al-4V

Ø	H		cod	€
4		1	NHSICN41	58
4		2	NHSICN42	58
4		3	NHSICN43	58
4		4	NHSICN44	58



Ø	H		cod	€
4,1	18°	0/2	NHSICN518	95
4,1	30°	0/2	NHSICN532	95
4,1	30°	2/4	NHSICN534	95



Mounter and S1BRS2 screw included

Mounter included

Tighten with HDH20 driver (page 58)

BALL ABUTMENTS Material: Ti-6Al-4V • CAH and CAT included

Ø	H		cod	€
4		1	NHSICN61	58
4		2	NHSICN62	58
4		3	NHSICN64	58



TIN Treatment on the gold part

Tighten with MDS or MDL screwdriver (page 59)

cod	€
CAH	16



Containment ring


cod	€
CALT	8



Nylon containment cap

IRETOR accessories page 37

H	cod	€
0	NHSICN80	100
1	NHSICN81	100
2	NHSICN825	100
3	NHSICN835	100
4	NHSICN845	100
6	NHSICN865	100



Tighten with 8393 screwdriver (page 60)

TIN Treatment on the gold part

Ring and cap not included

Ø 3.3 - 3.7 - 4.1 - 4.7 - 5.2

COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V


code	€
NHSICNDIA	27



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1BRS1


	code	€
standard	NHSICNSA	68
long	NHSICNSAL	68



T-BASE

Material: Ti-6Al-4V • Screw included: S1BRS1

	H	code	€
not rotating	1	NHSICN11DTB	79
not rotating	2	NHSICN12DTB	79
not rotating	4	NHSICN14DTB	79
rotating	1	NHSICN11DTBR	79
rotating	2	NHSICN12DTBR	79
rotating	4	NHSICN14DTBR	79




	cod	€
On request	S1BRS1T6	16



LINK

Material: Ti-6Al-4V

Ø	H	code	€
3.5	2	NHSICNL3502	89
3.5	3	NHSICNL3503	89
4.1	2	NHSICNL4102	89
4.1	3	NHSICNL4103	89



IRETOR ACCESSORIES

Components for the ball abutments of the lines **SVB, NHSI, S1B, NHSE** and **NHSIC**



ANALOG

Qty	code	€
2	144ATP	26



Material: Inox

TRANSFER

Qty	code	€
2	044CAIP	26



Material: Inox - PA

INSERTION TOOL

code	€
488EIP	47



CONTAINER IN TITANIUM

Qty	code	€
2	141CTP	29



Material: Ti-6Al-4V

CAP FOR LAB USE

Qty	code	€
4	143CPN	32



Material: PA

PARALLELE CAPS

Qty	pin	Kg	code	€
4	extra soft	0,7	142CPPG	31
4	soft	0,9	142CPPR	31
4	standard	1,5	142CPPT	31
4	strong	1,8	142CPPV	31




Material: PA

SET

code	€
192CPC	39

Set of copings with pins



Material: Ti-6Al-4V - PA - EVA

DISPARALLELE CAPS

Qty	pin	Kg	code	€
4	extra soft	0,6	143CPG	31
4	soft	0,8	143CPR	31
4	standard	1	143CPT	31
4	strong	1,5	143CPV	31



Material: PA

SET

code	€
192CPS	39


Set of copings without pins



Material: Ti-6Al-4V - PA - EVA

MUA COMPONENTS

Components for the mua abutments of the lines **SVB, NHSI, S1B, NHSE** and **NHSIC**

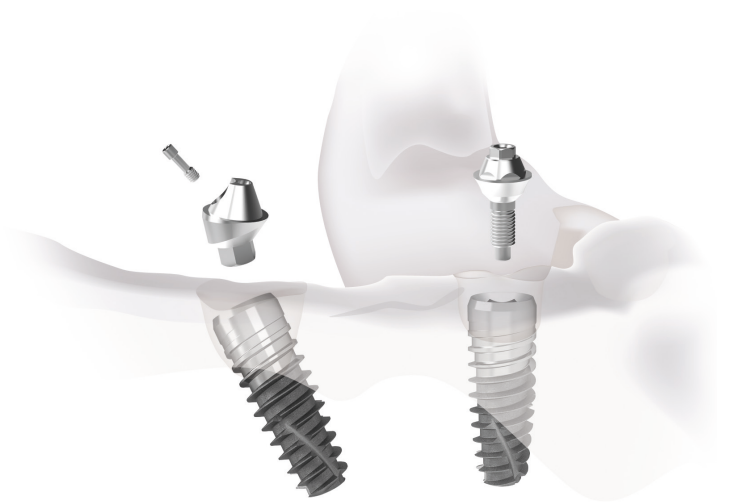

RETAINING SCREWS

Material: Ti-6Al-4V

cod	€
S1BRS3	16

For abutment thread 1.4



cod	€
S1BDTRSA	17

Long retaining screw for MUA transfer thread 1.4



HEALING CAPS

Screw included: S1BRS3

cod	€
S1BHCSRA	26

Material: Ti-6Al-4V



cod	€
S1BHCSRAA	26

Material: POM-C



ANALOG

Material: Ti-6Al-4V

cod	€
S1BIASRA	22



IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1BRS3

Material: Ti-6Al-4V • Screw included: S1BDTRSA

cod	€
S1BITCSRA	58

Indirect impression transfer



cod	€
S1BDTCSRA	37

Direct impression transfer. With long screw



ABUTMENT

Material: Ti-6Al-4V • Screw included: S1BRS3

cod	€
S1BPTTA	58

Temporary straight abutments



cod	€
S1BTTA	58

Definitive straight abutments



cod	€
S1BPCC	30

Castable abutments
Material: POM



cod	€
S1BTS	58

Abutments for welded technique



THREADED

Material: Ti-6Al-4V • Screw included: S1BRS3

cod	€
S1BTAE	58

Threaded not rotating



cod	€
S1BTAFB	58

Threaded abutment for bar



COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

cod	€
S1BDIASRA	22



SCAN ABUTMENT

Material: Ti-6Al-4V

cod	€
S1BSAA	58

Screw included: S1BRS3



T-BASE


Material: Ti-6Al-4V • Screw included: S1BRS3

cod	€
S1BTTADTB	68

Rotating



TISSUE LEVEL IMPLANTS

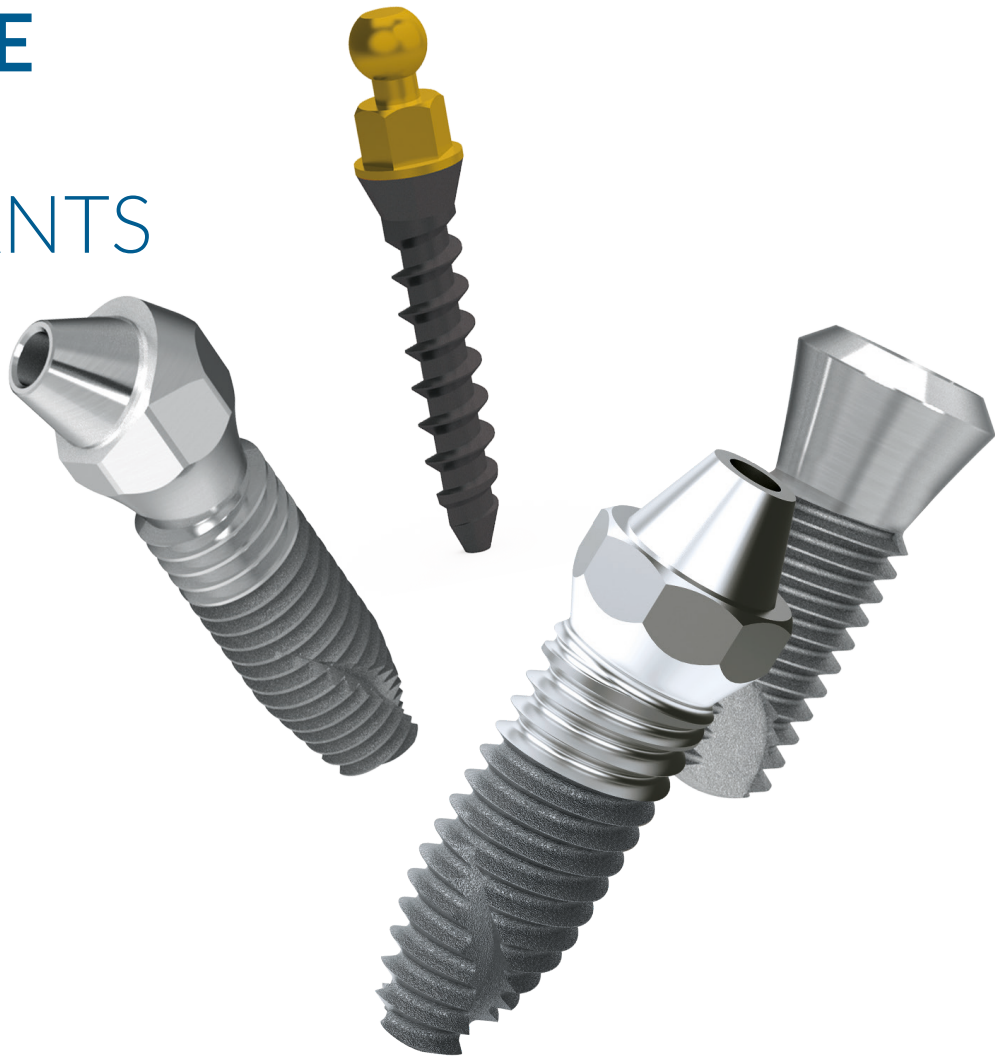

SHAPEONE

- INTERNAL OCTAGON \varnothing 3.7 - 4.1 - 4.7
- INTERNAL HEX \varnothing 3.7 - 4.1 - 4.7




iMAXMUA

- ONE PIECE \varnothing 3.3 - 3.7 - 4.1



SHAPEMINI


- SINGLE THREAD \varnothing 2.7



Dental implants are made of titanium for medical use in compliance with current regulations.

SHAPEONE

EXCELLENT PRIMARY STABILITY
ALSO IN BONE D4

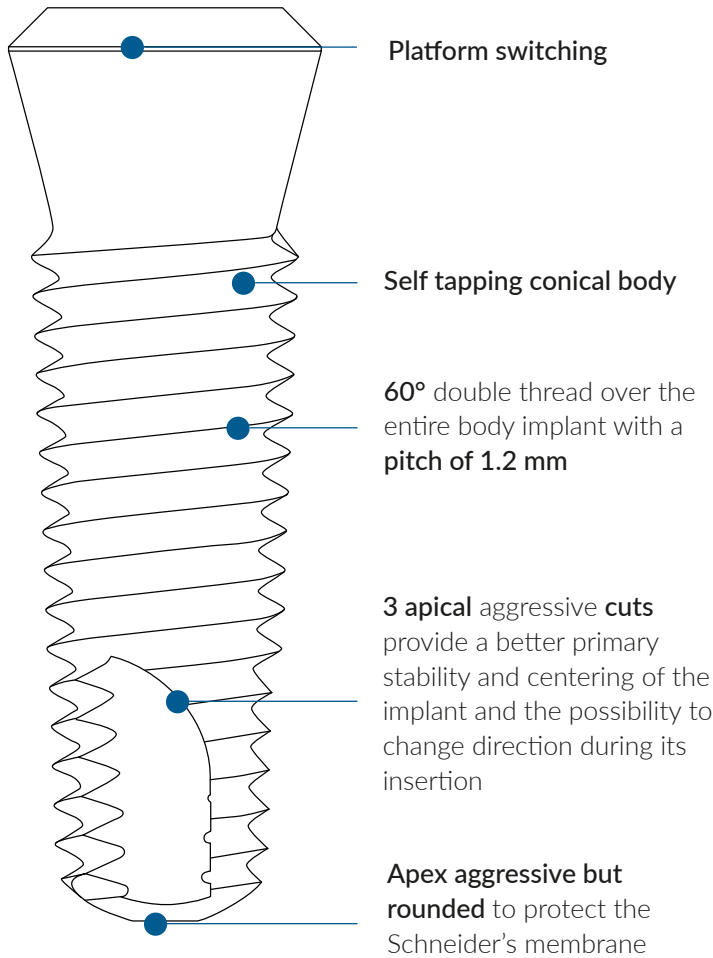

S1T-C
NECK MACHINED
€ 158

Mounter S1T1A50 included



Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	octagon (mm)	thread	
3.7			8	10	11.5	13	fine double thread 0.6	internal octagon	4.8	3.1	2	
4.1	4.5	6.5	8	10	11.5	13						16
4.7	4.5	6.5	8	10	11.5	13						16

DRIVERS

H	cod	€
25	HDH31S	47
30	HDH31L	47


Material: Surgical steel



PROSTHETIC COMPONENTS

IMPLANT CONNECTION

For the **S1T** line with internal **octagonal connection**, prosthetic components with cone inclined at 8° have been developed that prevent bacterial infiltration between implant and abutment.



INTERNAL OCTAGON
 8° angle on the implant and on the abutment

SURGICAL SCREWS

Material: Ti-6Al-4V

∅	H	code	€
4.8	2	S1TCS	16
4.8	5	S1TCSH	16



Available as spare parts
 S1TCS screw included

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1TRS1	16

For abutment thread 2 mm



code	€
S1TRS2	16

For abutment thread 2 mm



code	€
S1TDTRS	16

Long for transfer thread 2 mm



code	€
S1TRS1T6	16

Torx screw for digital



ANALOG

Material: Ti-6Al-4V

code	€
S1TIA	22



IMPRESSION TRANSFER

Material: Ti-6Al-4V

∅	code	€
5	S1T1A50	58

Multifunction abutment
 Indirect impression transfer
 Screw included: S1TRS1



∅	code	€
5	S1T1A50L	58

Multifunction abutment
 Direct impression transfer
 Screw included: S1TDTRS



CASTABLE ABUTMENTS

Material: POM-C + Ti-6Al-4V • Screw included: S1TRS1

∅	code	€
5	S1T3PC50	30

Non rotating



∅	code	€
5	S1T3PCR50	30

Rotating



ABUTMENTS

Material: Ti-6Al-4V

∅	code	€
4,5	S1T140	79

Straight conometric connection abutment
 Screw included: S1TRS1



∅	code	€
4,5	S1T240	89

20° angled conometric connection abutment
 Screw included: S1TRS2



BALL ABUTMENTS Material: Ti-6Al-4V • CAH and CALT included

∅	H	code	€
4,5	0	S1T60	47
4,5	1	S1T61	47
4,5	2	S1T62	47

TIN Treatment on the gold part
 Tighten with MDS or MDL screwdriver (page 59)



code	€
CAH	16

Containment ring



code	€
CALT	8

Nylon containment cap



COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

code	€
S1TDIA	22



SCAN ABUTMENT

Material: Ti-6Al-4V • Screw included: S1TRS1

code	€
S1TSA	58



T-BASE

Material: Ti-6Al-4V • Screw included: S1TRS1

	code	€
not rotating	S1T1DTB	79
rotating	S1T1DTBR	79




	code	€
On request	S1TRS1T6	16



SHAPEONE

EXCELLENT PRIMARY STABILITY
ALSO IN BONE D4

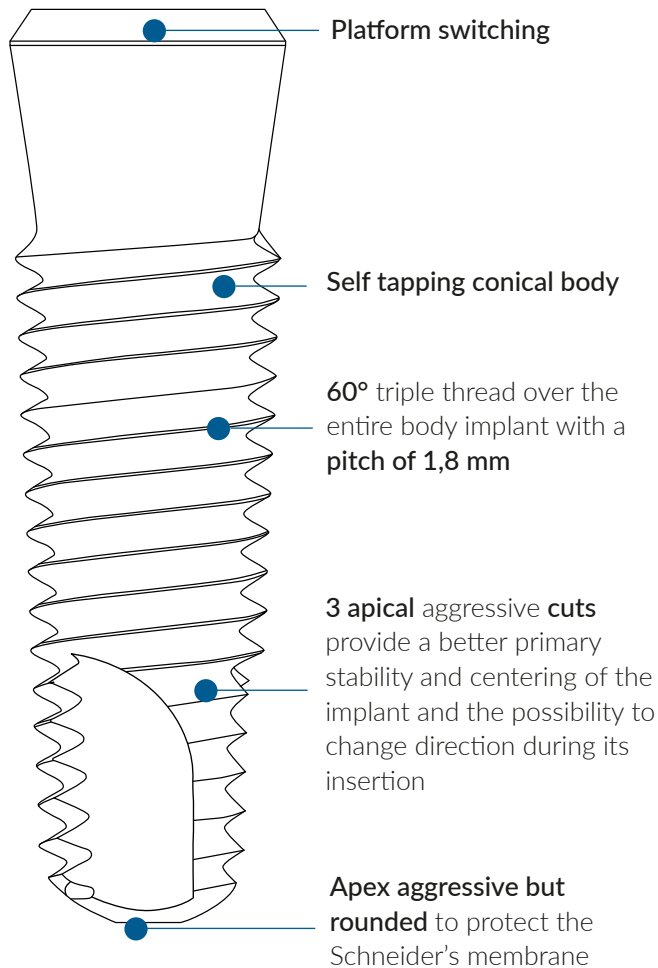

SHAPEONE TN C

S1TN-C
NECK MACHINED

€ 158



Ø	heights (mm)						implant thread (mm)	connection	platform (mm)	hex (mm)	thread	
3.7			8	10	11.5	13	16	fine triple thread 0.6	internal hex	3.5	2.5	1/72
4.1	4.5	6.5	8	10	11.5	13	16					
4.7	4.5	6.5	8	10	11.5	13	16					

DRIVERS

H	cod.	€
25	HDH25S	47
30	HDH25L	47

Material: Surgical steel




PROSTHETIC COMPONENTS

IMPLANT CONNECTION

Prosthetic components with **Friction Fit** connection have been developed for **S1TN** implant systems with **internal hex** connection. This connection ensures a “**cold fusion**” between implant and abutment if the retaining screw has been tightened at 30 Ncm. It eliminates micro movements and reduces bacterial infiltration between implant and abutment.

The S1TN implant prosthetic is compatible with the S1B, NHSI and SVB implant prosthetic (page 17-21)



UNIKO Friction Fit
 connection with 1° angle on the abutment

PROSTHETIC SCREWS

Material: Ti-6Al-4V

code	€
S1BRS1	16

For abutment thread 1/72



code	€
S1BDTRS	16

Long for transfer thread 1/72



ANALOG

Material: Ti-6Al-4V

∅	code	€
3.7	S1TNIA37	23
4.1	S1TNIA41	23
4.7	S1TNIA47	23



DIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1BDTRS

∅	code	€
3.5	S1TN1A35L	58
3.7	S1TN1A37L	58
4.1	S1TN1A41L	58
4.7	S1TN1A47L	58

Mounter transfer definitive straight abutment



INDIRECT IMPRESSION TRANSFER

Material: Ti-6Al-4V • Screw included: S1BRS1


∅	code	€
3.5	S1TN1A35	58
3.7	S1TN1A37	58
4.1	S1TN1A41	58
4.7	S1TN1A47	58

Mounter transfer definitive straight abutment





ONEPIECE
FOR IMMEDIATE LOADING

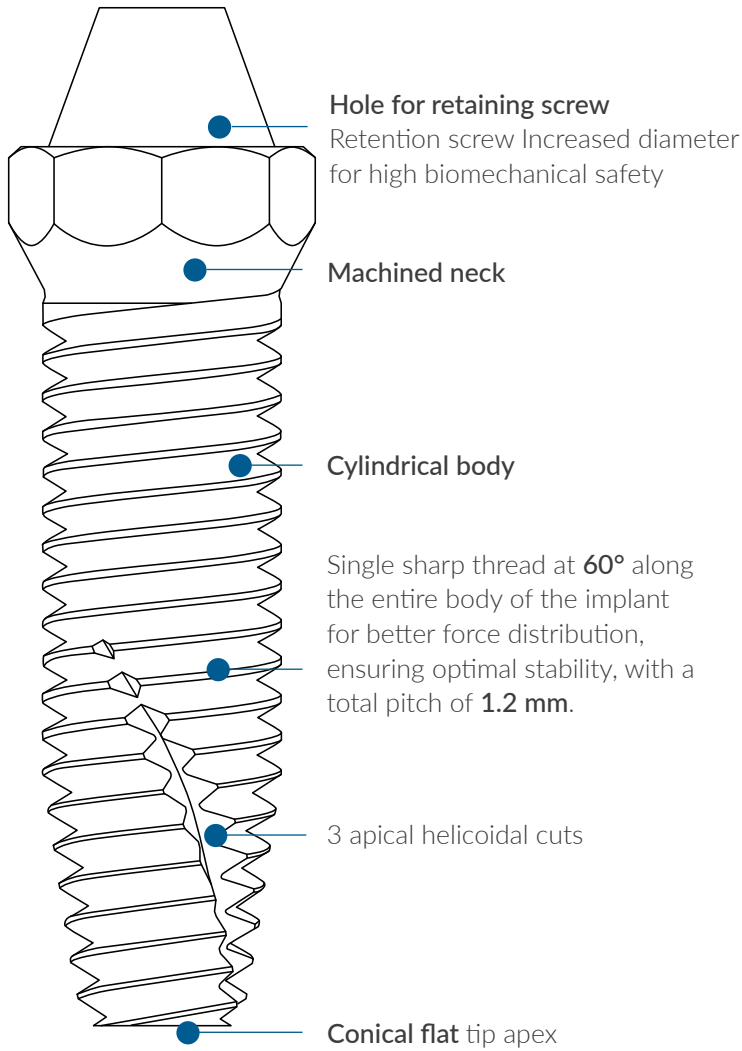

NHSM00-HYHA
HYBRID IMPLANT 0°
€ 210

Mounter NHSM included



NHSM18-HYHA
HYBRID IMPLANT 18°
€ 242



NHSM30-HYHA
HYBRID IMPLANT 30°
€ 242



Ø		heights (mm)					
3.3	0°	4.5	6	8	10	11.5	13
3.7	0°	4.5	6	8	10	11.5	13
4.1	0°	4.5	6	8	10	11.5	13
implant thread (mm)		connection		platform			
double		one piece		4.3			

Ø			implant thread (mm)			spira
3.7	18°	30°	11,5	13	16	double
4.1	18°	30°	11,5	13	16	double
connection (mm)			platform			
one piece			4.3			

DRIVERS

code	€
NHSMHDH	47


Implant driver
Material: Surgical steel



PROSTHETIC COMPONENTS

IMPLANT CONNECTION

There is no connection between implant and abutment in **NHSM ONEPIECE** system and this allows to **completely eliminate bacterial infiltration**. OnePiece connection is suitable for immediate loading.



ONE PIECE
 No connection
 between implant
 and abutment

RETAINING SCREWS

Material: Ti-6Al-4V

code	€
NHSMRS1	16



For abutment thread 1/72

code	€
NHSMDTRS	16



Long for transfer thread 1/72

HEALING CAPS

Screw included: NHSMRS1

code	€
NHSMHCSRA	26



Material: Ti-6Al-4V

code	€
NHSMHCSRAA	26



Material: POM-C

ANALOG

Material: Ti-6Al-4V

code	€
NHSMIASRA	22



IMPRESSION TRANSFER

Material: Ti-6Al-4V

code	€
NHSMITCSRA	58



Indirect
 Screw included: NHSMRS1

code	€
NHSMDTCSRA	37




Direct
 Screw included: NHSMDTRS

THREADED


Material: Ti-6Al-4V • Screw included: NHSMRS1

code	€
NHSMTTAE	58



Threaded not rotating

cod	€
NHSMTTAFB	58




Threaded abutments for bar

ABUTMENT

Material: Ti-6Al-4V • Vite inclusa: NHSMRS1


cod	€
NHSMPTTA	58

Temporary straight abutments



cod	€
NHSMTTA	58

Definitive straight abutments




cod	€
NHSMPPC	30

Castable abutment



cod	€
NHSMTS	58

Abutments for welded technique



COMPONENTS FOR DIGITAL FLOW

Implant libraries available on the site <https://www.en.ires.dental/media-kit/>

DIGITAL ANALOG

Material: Ti-6Al-4V

cod	€
NHSMDIASRA	22



SCAN ABUTMENT

Material: Ti-6Al-4V

cod	€
NHSMCAA	58


Screw included: NHSMRS1




T-BASE

Material: Ti-6Al-4V • Screw included: NHSMRS1

cod	€
NHSMTTADTB	68



SHAPEMINI

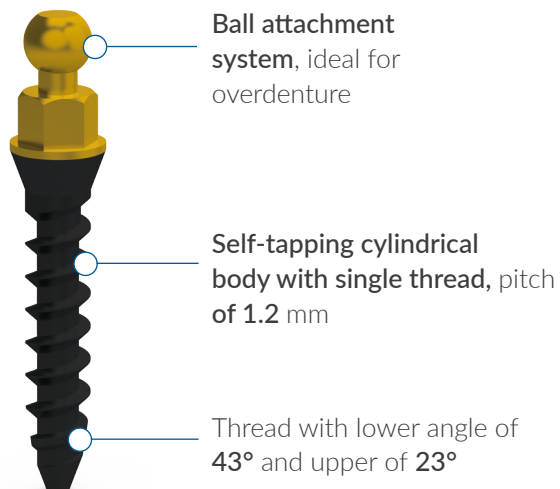

Ball attachment system, ideal for overdenture

Self-tapping cylindrical body with single thread, pitch of 1.2 mm

Thread with lower angle of 43° and upper of 23°



SM27YY

YY=HEIGHT

TIN BALL ATTACHMENT SYSTEM

€ 58

Ø	heights (mm)					Implant thread	connection
2,7	8	10	11.5	13	16	single	TIN ball attachment

COMPONENTS PROSTHETIC

ANALOGO

Material: Ti-6Al-4V

code	€
SMIA	22



CASTABLE ABUTMENT

Material: POM-C

code	€
SMC	30



code	€
CAH	16




Containment ring

code	€
CALT	8



Nylon containment cap

SELF-TAPPING IMPLANT WITH SINGLE THREAD

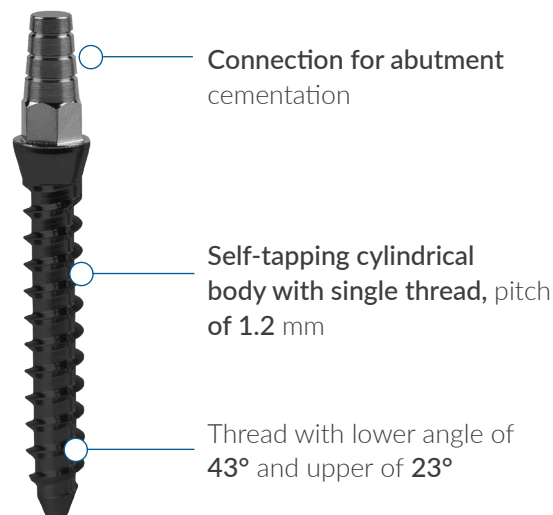

Connection for abutment cementation

Self-tapping cylindrical body with single thread, pitch of 1.2 mm

Thread with lower angle of 43° and upper of 23°



SM27YYF

YY=HEIGHT

IMPLANT WITH FIXED ABUTMENT

€ 58

Ø	heights (mm)					Implant thread
2,7	8	10	11.5	13	16	single

COMPONENTS PROSTHETIC

ANALOGO

Material: Ti-6Al-4V

cod	€
SMIAF	22



STRAIGHT ABUTMENT

Material: POM-C

code	€
SMF	30



IMPLANT SYSTEMS

SURFACE TREATMENT

There is a relevant scientific literature* on how surface roughness characteristics influence cell behaviour. Compared to a smooth surface, topographical patterns smaller in size than a fibroblast cell (micro and nano topography) orient the arrangement of the cells and stimulate osteoblastic and platelet activity, accelerating the production of extracellular matrix and bone regeneration, and therefore the osseointegration of the dental implant.

The three **fundamentals of surface treatment of dental implants** from a biological point of view are:

1. **control of surface topography** to stimulate cellular response in an osteogenic direction;
2. **control of the chemical composition of the surface** to promote cell colonization;
3. **control of biological contamination** from adherent endotoxins so as not to interfere with the natural inflammatory response.

For the surface treatment a sand-blasting process was used followed by a double acid attack. In the images, increasing the magnification, it can be seen how the macroscopic aspects of the screw (spire, cutting SLA surface treatment edge) are not affected by the treatment and that the surface is free from processing residue. The dual-beam roughness typical of SLA treatment can be clearly observed, which contains large cavities due to large grit blasting on which is superimposed the micro-roughness due to treatment


with acids. The micro-roughness illustrated in the figures highlights the typical three-dimensional topography, which gives these surfaces “sponge-like” characteristics that are the basis of their excellent clinical performance. In fact, the very short peak-to-peak distance, about 1 micrometer, stimulates both the activity of osteogenic cells and the capillary penetration of the blood in the surface structure, offering very favorable characteristics to stimulate bone regeneration, as described in many articles on this topic. This unique combination of long-range roughness (large grit sand-blasting) and short-range (acid etching) is a substrate favorable to cell regrowth that adequately promotes cell differentiation.

The level of roughness is Ra 1.42 ± 0.12.


HYHA

HYBRID IMPLANT


Partial surface treatment on the body implant with hyaluronic acid. Cold plasma decontamination*




MAG 52 X
WD 11.5 mm
EHT 20.00 kV
Signal A CZ BSD




MAG 200 X
WD 11.0 mm
EHT 20.00 kV
Signal A CZ BSD



MAG 1.50 K X
WD 11.5 mm
EHT 20.00 kV
Signal A SE1



Sa 0,50 µm
overall mean value on a measuring area of 30x30 µm
cold plasma decontamination




Sa 1,90 µm
overall mean value on a measuring area of 30x30 µm
sand-blasting, double etching, cold plasma decontamination

C

NECK MACHINED

Surface treatment on the body implant

* Valutazione della composizione chimica superficiale, della morfologia, della citotossicità e dell'adesione cellulare su impianti dentali. G. Cascardo, C. Cassinelli, Doctor OS 2005 Nov-Dic; 16 (9): 1091. Valutazione comparativa del trattamento di superficie in 5 sistemi implantari. M. Biasotto, M. Cadenaro et al. Università degli studi di Trieste. Quintessence International, Anno 18 - Maggio/Giugno 2002. RAPPORTO ISTISAN 01/15 - Valutazione del trattamento superficiale sulle prestazioni meccaniche a fatica di impianti in titanio plasma-sprayed e titanio sabbato e mordenzato. Rossella Bedini, Giorgio de Angelis, Marco Tallarico, Rosario Ialpi, Umberto Romeo, Giuseppe di Cintio 2001, 33 p. RAPPORTO ISTISAN 08/32 - Valutazione microtomografica dell'area di possibile contatto osseo di sei tipologie diverse di impianti dentali. Rossella Bedini, Raffaella Pec-ci, Fabio Di Carlo, Alessandro Quaranta, Francesca Rizzo, Manlio Quaranta, G. Heimke, W. Schulte, B. d'Hoedt, P. Griss, C.M. Büsing, D. Stock. The influence of fine surface structures on the osseointegration of implants. The International Journal of Artificial Organs 1982; 5(3): 207-212. Guy, M.J. McQuade, M.J. Scheidt, J.C. McPherson III, J.A. Rossmann, T.E. Van Dyke. In vitro attachment of human gingival fibroblasts to endosseous implant materials. Journal of Periodontology 1993 Jun; 64(6): 542-546.

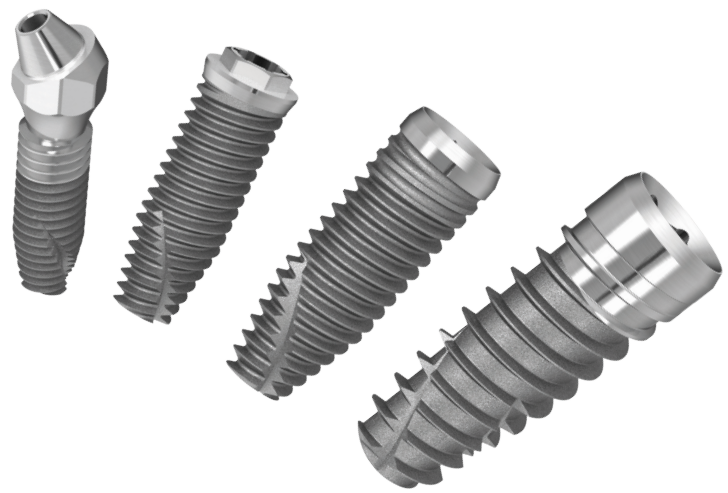


CYTOTOXICITY TEST

EN ISO 10993-5: 2009

Valutazione Biologica dei Dispositivi Medici

Prove per la citotossicità in vitro

After treatment and decontamination, the implants proved to be perfectly cytocompatible, that is devoid of cytotoxic effects against L929 fibroblasts. In all wells, the cells always showed density and morphology fully comparable with those of the negative control. The fibroblasts proliferate homogeneously in contact with the implants as the Material does not release any cytotoxic element. Moreover, multinucleated giant cells were never shown in significantly higher number than the negative control, indicating the absence of effects of an inflammatory type.

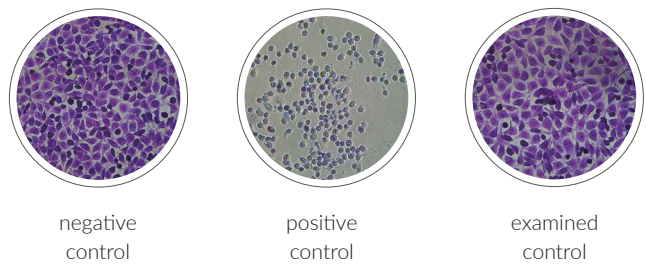

COLD PLASMA DECONTAMINATION

After the surface treatment, the implants are cleaned to remove processing residues by washing them with solvents and then subjecting them to a process of surface decontamination with cold plasma (Argon). The partially ionized Argon atoms (inert gas) act as an additional atomic sand-blasting that promotes the removal of organic contaminants and activates the ionization of surface atoms of titanium, improving the wettability of the implant. The treatment conditions adopted on shape1 implants offer

the best characteristics considered important, according to the state of current knowledge*, in the processes of implant healing, both in terms of surface morphology and in terms of chemical composition (surface cleaning). Plasma cleaning, packaging in a controlled environment, the absolute respect of “clean” procedures, quality control tests of during the manufacturing process, play a fundamental role in the control of adherent endotoxins (biological cleaning), the main agent of immunological response to implant surfaces.

* Valutazione del rapporto tra costo e qualità della pulizia superficiale di alcuni sistemi implantari in commercio Marco Morra, Clara Cassinelli, Giovanna Cascardo, Daniele Bollati, Nobil Bio Ricerche srl Via Valcastellana 26, 14037, Portacomaro (AT)
M. Morra, C.Cassinelli, Evaluation of Surface Contamination of Titanium Dental Implants by Lu-Sem: Comparison with XPS Measurements Surface and Interface Analysts, Vol. 25, 983-984 (1997).

STERILIZATION & PACKAGING

To preserve its integrity, the dental implant is housed in a vertical position inside a titanium cylinder anchored, by means of the closing cap, to the respective vial made of borosilicate glass for pharmaceutical use, complying with the European Pharmacopoeia in force. This vial really ensures the neutrality of the primary packaging due to the absence of release of contaminants during the sterilization phase. It is inserted in a blister of transparent polyglass sealed with heat-sealing lacquer-based Tyvek and packed in a cardboard box that also

contains the instructions for use and the labels for the patient records, on which are printed the data that allow product traceability (code and batch number). All the product packaging Materials have been tested, approved and certified. Implants are supplied sterile, in a pack that allows their stability to be guaranteed for 5 years. The sterilization process is performed with gamma rays respecting the standards in force by qualified suppliers who use automated, safe and reliable systems, with continuous microbiological monitoring of the process.

SURGICAL KIT

ONE SURGICAL KIT FOR ALL THE IMPLANT SYSTEMS


The purpose of **surgical trays** is to store the instruments used to insert dental implants. The kit can be **carried**, **sterilized** and **kept** in a horizontal position with the lid closed. All the instruments must be cleaned and sterilized before the first use.

The surgical kit and instruments are not sterile at the time of delivery.
The standard kits contain connectors for internal hexagon: connectors for other connections are available upon request.

CSK SURGICAL KIT

code	€
CSK	2.625

code	description
DE	drill extender
LD	lance drill
D20M	pilot drill ø 2.0
D2024M	drill ø 2.0 2.4 mm
CSD33	countersink ø 3.3
D2428M	drill ø 2.4 2.8 mm
CSD37	countersink ø 3.7
D2833M	drill ø 2.8 3.3 mm
CSD41	countersink ø 4.1
D3338M	drill ø 3.3 3.8 mm
CSD47	countersink ø 4.7
D3844M	drill ø 3.8 4.4 mm
CSD52	countersink ø 5.2
D4448M	drill ø 4.4 4.8 mm
DS43341M	stop 4.5
DS63341M	stop 6.5
DS83341M	stop 8
DS103341M	stop 10
DS113341M	stop 11.5
DS133341M	stop 13
TWA4	complete ratchet
THDDS	short contra-angle screwdriver for hexagon 1.25 mm
THDDL	long contra-angle screwdriver for hexagon 1.25 mm
HDH21S	connectors short for internal hex 2.1
HDH21L	connectors long for internal hex 2.1
HDH25S	connectors short for internal hex 2.5
HDH25L	connectors long for internal hex 2.5
PP	parallel pin 0°

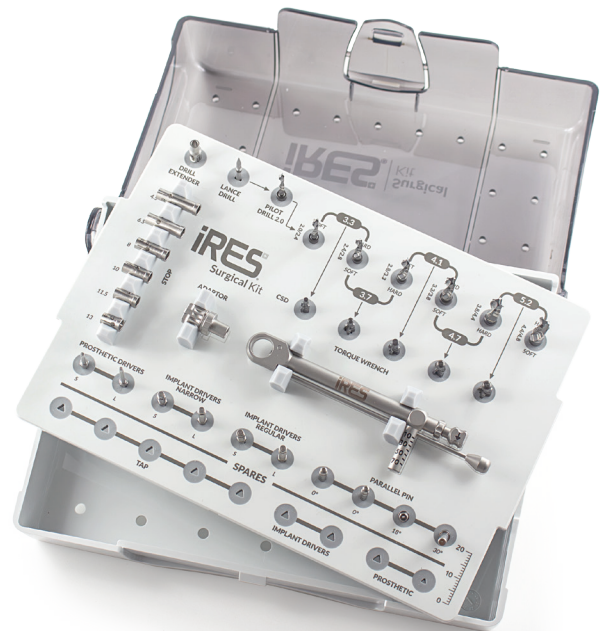

SMALL SURGICAL KIT



COMPLETE

	<i>cod</i>	€
	Ergo Kit Complete	2.980

<i>code</i>	<i>description</i>
LD	lance drill
D20M	pilot drill \varnothing 2.0
D2024M	drill \varnothing 2.0 2.4 mm
CSD33	countersink \varnothing 3.3
D2428M	drill \varnothing 2.4 2.8 mm
CSD37	countersink \varnothing 3.7
D2833M	drill \varnothing 2.8 3.3 mm
CSD41	countersink \varnothing 4.1
D3338M	drill \varnothing 3.3 3.8 mm
CSD47	countersink \varnothing 4.7
D3844M	drill \varnothing 3.8 4.4 mm
CSD52	countersink \varnothing 5.2
D4448M	drill \varnothing 4.4 4.8 mm
HDH21L	connectors long for internal hex 2.1
HDH25L	connectors long for internal hex 2.5
TWA4	complete ratchet
DE	drill extender
TAPXXX33*	tap \varnothing 3.3
TAPXXX37*	tap \varnothing 3.7
TAPXXX41*	tap \varnothing 4.1
TAPXXX47*	tap \varnothing 4.7
TAPXXX52*	tap \varnothing 5.2
PP	parallel pin 0°
THDDS	short contra-angle screwdriver for hexagon 1.25 mm
THDDL	long contra-angle screwdriver for hexagon 1.25 mm
HDH21S	connectors short for internal hex 2.1
HDH25S	connectors short for internal hex 2.5
MDS	short manual screwdriver for hexagon 1.25 mm
MDL	long manual screwdriver for hexagon 1.25 mm
MDLAA	manual screwdriver for angled torx
DS43341M	stop 4.5
DS63341M	stop 6.5
DS83341M	stop 8
DS103341M	stop 10
DS113341M	stop 11.5
DS133341M	stop 13

*choice of Shapeone or iMAX

BASIC

	<i>cod</i>	€
	Ergo Kit Basic	1.880

<i>code</i>	<i>description</i>
LD	lance drill
D20M	pilot drill \varnothing 2.0
D2024M	drill \varnothing 2.0 2.4 mm
CSD33	countersink \varnothing 3.3
D2428M	drill \varnothing 2.4 2.8 mm
CSD37	countersink \varnothing 3.7
D2833M	drill \varnothing 2.8 3.3 mm
CSD41	countersink \varnothing 4.1
D3338M	drill \varnothing 3.3 3.8 mm
CSD47	countersink \varnothing 4.7
D3844M	drill \varnothing 3.8 4.4 mm
CSD52	countersink \varnothing 5.2
D4448M	drill \varnothing 4.4 4.8 mm
THDDL	long contra-angle screwdriver for hexagon 1.25 mm
HDH21L	connectors long for internal hex 2.1
HDH25L	connectors long for internal hex 2.5
TWA4	complete ratchet

PROSTHETIC KIT

PSK PROSTHETIC KIT

code	€
PSK	945

code	description
MDXS	extra short manual screwdriver for hexagon 1.25 mm
MDS	short screwdriver hex 1.25 mm
MDL	long screwdriver hex 1.25 mm
MDLAA	angled torx hand screwdriver
TRT	removal tool for abutments
MTRT	manual abutment extractor
HDH20	Implant driver for straight MUA
HDH25M	connector for Shape Mini
THDDS	short prosthetic screwdriver hex 1.25
THDDL	long prosthetic screwdriver hex 1.25
THDDAL	angled torx contra-angle screwdriver
TWA4	ratchet wrench



PROCEDURA PER LA GESTIONE DEI KIT


CLEANING

1. **Dismantle** all the compound parts.
2. **Rinse** abundantly with cold or lukewarm water for **2-5 minutes**.
3. Leave the instruments for **10 minutes** in an **ultrasonic** cleaner with a neutral pH enzymatic detergent diluted in water according to the product instructions.
4. **Wash** the instruments with water for **3 minutes**.

STERILIZATION

The guidelines for sterilization are listed below. Exceeding these sterilization limits may cause deterioration of the plastic components.

Type of cycle (value)	Temperature (°C - F)	Exposure	Drying time
Pre-vacuum	132 / 270	3 minutes	30 minutes
Pre-vacuum	134 / 273	18 minutes	30 minutes
Gravity	121 / 250	80 minutes	30 minutes

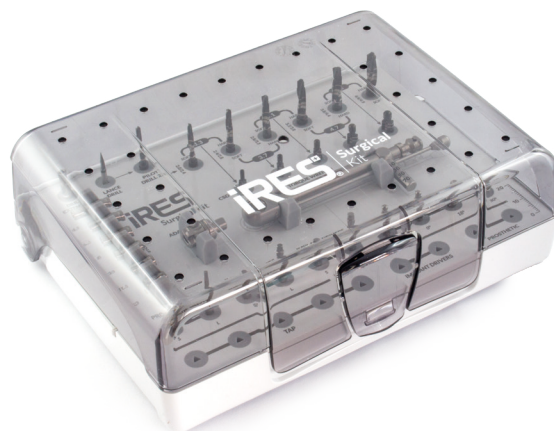


DRILLS

For a proper osteotomy and to maintain the integrity of bone quality, the maximum recommended speed is 800rpm with direct input on drill of saline solution to facilitate cooling. All drills are made of medical stainless steel and subjected to hardening heat treatment. Maximum recommended number of use of the devices 30 times. The helical milling cutters have reference laser markings that identify the depth to reach, until 8 mm with a thin white line, from 10 to 13 mm with a white band in which at half is identified the 11.5 mm height, and finally a thin white line for the 16 mm. This system gives a clear and intuitive glance of the depth level reached by the drill. 4.5 and 6.5mm are not present to avoid confusion in reading the demarcation lines, and being these measures close to the nerve, it is always recommended to use stop by 4.5 and 6.5 mm.

The drills from 2.0 to 2.8/3.3 have a **sharp apex**, The drills from 33/38 - 38/44 - 44/48 have a **flat apex**, they do not increase the height of the cut, but are only used to widen the osteotomy.

They must not be used for cutting, but as an aid for inserting the implant

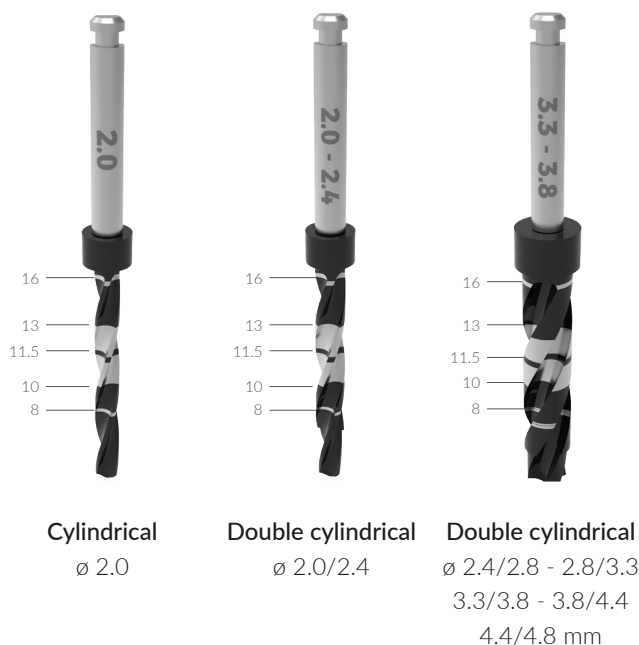

Cylindrical ø 2.0	Double cylindrical ø 2.0/2.4	Double cylindrical ø 2.4/2.8 - 2.8/3.3 3.3/3.8 - 3.8/4.4 4.4/4.8 mm
----------------------	---------------------------------	--

DRILL EXTENDER

Material: Surgical steel



code	€
DE	42

LANCE DRILL Ø 2

Material: Surgical steel



code	€
LD	47

DRILLS H. 36







Material: Surgical steel



ø 2		ø 2.0 2.4		ø 2.4 2.8		ø 2.8 3.3		ø 3.3 3.8		ø 3.8 4.4		ø 4.4 4.8	
code	€	code	€	code	€	code	€	code	€	code	€	code	€
D20M	74	D2024M	74	D2428M	74	D2833M	74	D3338M	74	D3844M	74	D4448M	74

STOPS FOR DRILLS 2.0 - 2.0/2.4 - 2.4/2.8 - 2.8/3.3

Material: Ti-6Al-4V

					
h. 4.5	h. 6.5	h. 8	h. 10	h. 11.5	h. 13
code €	code €	code €	code €	code €	code €
DS43341M 37	DS63341M 37	DS83341M 37	DS103341M 37	DS113341M 37	DS133341M 37


The length of the stops ranges from **4.5 mm to 13 mm**.

The 33/38 - 38/44 - 44/48 cutters do not have stops as they are characterized by a flat tip.

COUNTERSINK

The countersinks are used when there is **the need to enlarge the initial part of the hole** created to adapt this shape to the neck of the implant to be inserted. **The maximum recommended speed is 300 rpm** with direct input on drill of saline solution to facilitate cooling. The countersink should be used in perfect axis with the osteotomy to avoid its ovalization in the coronal part. The countersinks present **two laser markings** that identify the depth to be reached on the basis of the bone consistency, at **1.4 mm for a "D3" bone, at 2.8 mm for both "D2" and "D1" bones**. Above the marking at 2.8 mm, the countersink continues with a cylindrical geometry that does not compromise the osteotomy although more deeply inserted.

∅ 3.3 - 3.7 - 4.1 - 4.7 - 5.2








for short implant








without insertion head for all sizes

COUNTERSINK

Material: Surgical steel


				
∅ 3.3	∅ 3.7	∅ 4.1	∅ 4.7	∅ 5.2
code €	code €	code €	code €	code €
CSD33 95	CSD37 95	CSD41 95	CSD47 95	CSD52 95

				
∅ 3.3	∅ 3.7	∅ 4.1	∅ 4.7	∅ 5.2
code €	code €	code €	code €	code €
CSDS33 95	CSDS37 95	CSDS41 95	CSDS47 95	CSDS52 95

TAPS

In very dense bone (Type I) it is recommended to use a tap with the same system profile to insert. The tap is sharper than the implant and it allows to prepare the implantation site with reduced trauma.

The maximum recommended speed is 30 rpm with direct input on tap of saline solution to facilitate cooling.



SHAPEONE TAPS

Material: Surgical steel



∅ 3.7

∅ 4.1

∅ 4.7

code €

code €

code €

TAPS1B37 95

TAPS1B41 95

TAPS1B47 95

IMAX TAPS

Material: Surgical steel



∅ 3.3

∅ 3.7

∅ 4.1

∅ 4.7

∅ 5.2

code €

code €

code €

code €

code €

TAPIMAX33 95

TAPIMAX37 95

TAPIMAX41 95

TAPIMAX47 95

TAPIMAX52 95

MUCOTOMI

Material: Surgical steel



∅ 3.3

∅ 4

code €



code €

HDHCSN 50

HDHCSR 50

CONNECTORS

In the kit all the connectors have a handpiece attack that may be used both in manual mode and with the ratchet, thanks to the special washer (WH2). The insertion torque for the **immediate loading** will be in the range **from 35 to 50Ncm**. For the **conventional** load the **insertion torque should never exceed 50Ncm**.

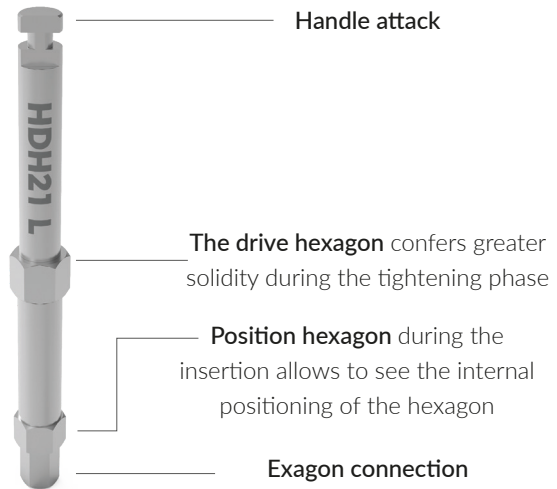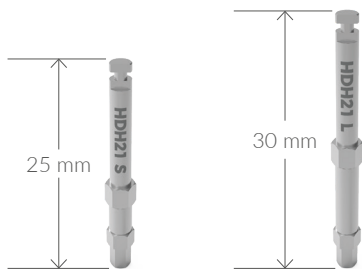

Exagon connection that reaches the stop of the system, has a steel retention ring reinforced and raised both to avoid interferences during the implant insertion and to reduce the wear of the retention

Material: Surgical steel

∅	h.	code	€
2,1	25	HDH21S	47
2,1	30	HDH21L	47

Internal hex narrow



∅	h.	code	€
2,5	25	HDH25S	47
2,5	30	HDH25L	47

For internal hex regular



∅	h.	code	€
2,4	25	HDH24S	47
2,4	30	HDH24L	47

External hex narrow



∅	h.	code	€
2,7	25	HDH27S	47
2,7	30	HDH27L	47

For external hex regular



∅	h.	code	€
3,1	25	HDH31S	47
3,1	30	HDH31L	47

For octagon



code	€
HDH20	47

For straight MUA



code	€
HDH25M	47

For Shape Mini



code	€
NHSMHDH	47

For iMAX MUA



ACCESSORIES

PARALLISM PIN

Material: Ti-6Al-4V



code	€
0°	
PP	21

ORIENTER POSITION

Material: POM-C e Ti

code	€
NHSMFL	22

For iMAX Mua



GUIDE TO DRILL INCLINATION

Material: Surgical steel

code	€
NHSMG	126

A 0° - 18° - 30°



DRIVERS AND SCREWDRIVERS

PROSTHETIC SCREWDRIVERS

Material: Surgical steel


	code	€
short	THDDS	47
long	THDDL	47

For hex 1.25 mm contra-angle connection



	code	€
extra short	MDXS	47
short	MDS	47
long	MDL	47

Manual screwdriver for hexagon 1.25 mm



	code	€
	MDLAA	68

Torx 1.25 mm manual angled



	code	€
	THDDAL	47

Angled torx contra-angle screwdriver



SCREWDRIVERS

Material: Surgical steel

code	€
IDL	68



code	€
8393	100

For iRetor



REMOVAL TOOLS

Material: Surgical steel

code	€
TRI	100

For implants



code	€
TRT	100

For abutments



code	€
MTRT	100

Manual abutment extractor



EXTRACTION KIT FOR RETAINING SCREWS

cod	€
D15RS	116

Drill
Material: Surgical steel



cod	€
GRS	63

Guide for drill
Material: Ti-6Al-4V



cod	€
SGRS	105

Holder for GRS
Material: Ti-6Al-4V



RATCHET

Material: Surgical steel

Reverse fixed ratchet: It allows to screw and unscrew without having to pull out and turn the adapter

Ratchet wrench: mounted on the reverse ratchet, it allows to measure up to 70Ncm without breaking the rod through the stop final race



Housing for 8mm washer to confer greater resistance to higher torque.



Under the 70Ncm is present a safety catch to prevent the leakage of the dragging arm, avoiding its breakage.



Reverse to change direction of unscrewing and screwing without having to remove and replace the ratchet.



Ratchet adaptor

ø 8 mm reinforced that adding solidity

code	€
WH2	53

Material: Surgical steel

code	€
TW4	242

Without adapter



code	€
TWA4	294

Complete



KIT SINUS LIFT

code	€
SINUS KIT	2.205

code	description
DE	drill extender
SD5	standard drill h 5 mm
SD6	standard drill h 6 mm
SD7	standard drill h 7 mm
SD8	standard drill h 8 mm
SPD	standard pilot drill
SPI	standard start drill
SBL	standard body lift
APD	advanced pilot drill
AID	advanced start drill
AD2	advanced drill h 2 mm
AD3	advanced drill h 3 mm
AD4	advanced drill h 4 mm
ABL	advanced body lift
RBL	ratchet body lift



SURGICAL PROTOCOL

DRIVERS- FINAL DRILLS- COUNTERSINKS - TAPS

heights from 8 to 16 mm

Implant system	Drivers	Ø	Finla drills (Bone d4)	Final drills (Bon d3-d2-d1)	CSD (Bone d3 - d2)	TAP (Bone d1)
iMAX NHSI 3.3	HDH21S HDH21L	3.3	D2024M	D2428M	CSD33	TAPIMAX33
SHAPEONE B	HDH25S HDH25L	3.7	D2428M	D2833M	CSD37	TAPS1B37
		4.1	D2833M	D3338M-P	CSD41	TAPS1B41
		4.7	D3338M-P	D3844M-P	CSD47	TAPS1B47
SHAPEONE Tn	HDH25S HDH25L	3.7	D2428M	D2833M	CSD37	TAPS1B37
		4.1	D2833M	D3338M-P	CSD41	TAPS1B41
		4.7	D3338M-P	D3844M-P	CSD47	TAPS1B47
iMAX NHSI	HDH25S HDH25L	3.7	D2428M	D2833M	CSD37	TAPiMAX37
		4.1	D2833M	D3338M-P	CSD41	TAPiMAX41
		4.7	D3338M-P	D3844M-P	CSD47	TAPiMAX47
		5.2	D3844M-P	D4448M-P	CSD52	TAPiMAX52
iMAX NHSIC Narrow	HDH21S HDH21L	3.3	D2024M	D2428M	CSD33	TAPIMAX33
		3.7	D2428M	D2833M	CSD37	TAPiMAX37
iMAX NHSIC Regular	HDH25S HDH25L	4.1	D2833M	D3338M-P	CSD41	TAPiMAX41
		4.7	D3338M-P	D3844M-P	CSD47	TAPiMAX47
		5.2	D3844M-P	D4448M-P	CSD52	TAPiMAX52
Volution SVB	HDH21S HDH21L	3.3	D2024M	D2428M	CSD33	
		3.7	D2428M	D2833M	CSD37	
	HDH25S HDH25L	4.1	D2833M	D3338M-P	CSD41	
		4.7	D3338M-P	D3844M-P	CSD47	
iMAX NHSE 3.3	HDH24S HDH24L	3.3	D2024M	D2428M	CSD33	TAPIMAX33
		3.7	D2428M	D2833M	CSD37	TAPiMAX37
iMAX NHSE	HDH27S HDH27L	4.1	D2833M	D3338M-P	CSD41	TAPiMAX41
		4.7	D3338M-P	D3844M-P	CSD47	TAPiMAX47
		5.2	D3844M-P	D4448M-P	CSD52	TAPiMAX52
		3.7	D2428M	D2833M	CSD37	TAPS1B37
SHAPEONE T (abutment included in the pack)	HDH25S HDH25L	4.1	D2833M	D3338M-P	CSD41	TAPS1B41
		4.7	D3338M-P	D3844M-P	CSD47	TAPS1B47
		3.7	D2428M	D2833M	CSD37	TAPS1B37
SHAPEONE T (after removing the abutment tighten the implant)	HDH31S HDH31L	4.1	D2833M	D3338M-P	CSD41	TAPS1B41
		4.7	D3338M-P	D3844M-P	CSD47	TAPS1B47
		3.7	D2428M	D2833M	CSD37	TAPS1B37
iMAXMUA 0°	NHSMHDH	3.3	D2024M	D2428M	CSD33	TAPIMAX33
iMAXMUA 18°	NHSMFL	3.7	D2428M	D2833M	CSD37	TAPiMAX37
iMAXMUA 30°	(driver)	4.1	D2833M	D3338M-P	CSD41	TAPiMAX41
SHAPEMINI	HDH25M	2.7	D20M	D2024M		

heights from 8 to 16 mm

SURGICAL PROTOCOL

∅ 3.7 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.7 countersink and 3.7 tap

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Countersink	Tap
Soft d4	•	•	•					
Medium d3/d2	•	•	•	•			•	
Compact d1	•	•	•	•			•	•

∅ 4.1 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink and 4.1 tap

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Countersink	Tap
Soft d4	•	•	•	•				
Medium d3/d2	•	•	•	•	•		•	
Compact d1	•	•	•	•	•		•	•

∅ 4.7 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.7 countersink and 4.7 tap

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Countersink	Tap
Soft d4	•	•	•	•	•			
Medium d3/d2	•	•	•	•	•	•	•	
Compact d1	•	•	•	•	•	•	•	•

Ø 3.3

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.3 countersink and 3.3 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Step	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Maschiatore
Bone									
Soft d4	•	•							
Medium d3/d2	•	•	•					•	
Compact d1	•	•	•					•	•

Ø 3.7

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.7 countersink and 3.7 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Step	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Maschiatore
Bone									
Soft d4	•	•	•						
Medium d3/d2	•	•	•	•				•	
Compact d1	•	•	•	•				•	•

Ø 4.1


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink and 4.1 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Step	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Maschiatore
Bone									
Soft d4	•	•	•	•					
Medium d3/d2	•	•	•	•	•			•	
Compact d1	•	•	•	•	•			•	•

ø 4.7


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Utilizzare Use 4.7 countersink and 4.7 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•	•	•				
Medium d3/d2	•	•	•	•	•	•		•	
Compact d1	•	•	•	•	•	•		•	•

ø 5.2


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 5.2 countersink and 5.2 tap

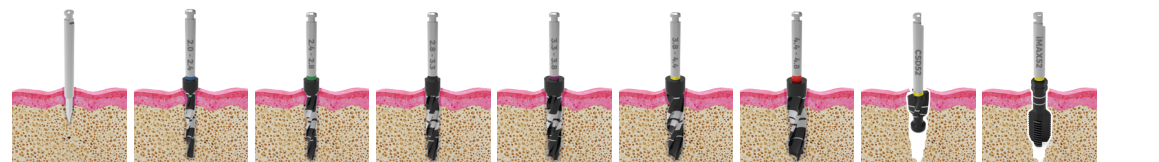

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•	•	•	•			
Medium d3/d2	•	•	•	•	•	•	•	•	
Compact d1	•	•	•	•	•	•	•	•	•


ø 3.3

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.3 countersink




	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•	•						
Medium d3/d2	•	•	•					•
Compact d1	•	•	•					•

Ø 3.7 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.7 countersink

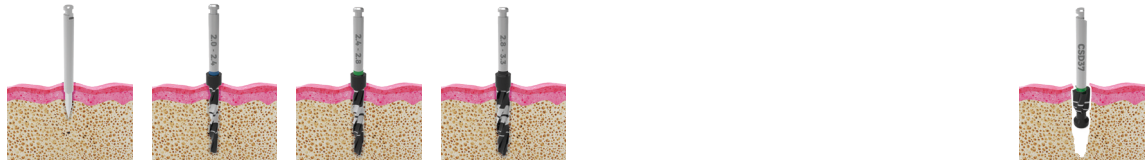


	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	●	●	●					
Medium d3/d2	●	●	●	●				●
Compact d1	●	●	●	●				●

Ø 4.1 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink

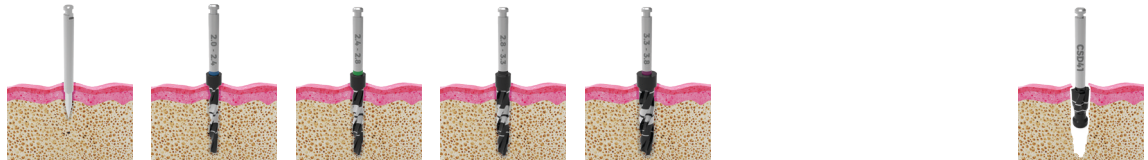


	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	●	●	●	●				
Medium d3/d2	●	●	●	●	●			●
Compact d1	●	●	●	●	●			●

Ø 4.7 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.7 countersink

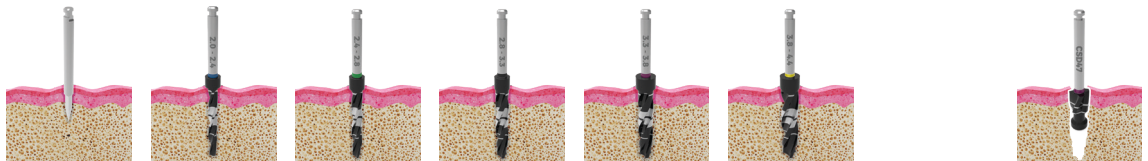

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	●	●	●	●	●			
Medium d3/d2	●	●	●	●	●	●		●
Compact d1	●	●	●	●	●	●		●

Ø 5.2 Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 5.2 countersink

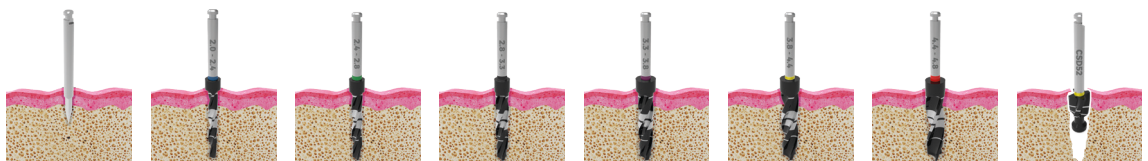


	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	●	●	●	●	●	●		
Medium d3/d2	●	●	●	●	●	●	●	●
Compact d1	●	●	●	●	●	●	●	●

Implant system	Drivers	Ø	Final drills (Bone d4)	Final drills (Bone d3-d2-d1)	CSD (Bone d3-d2)	TAP (d1 bone)
SHAPEONE B	HDH25S	4.1	D3338M-P	D3844M-P	CSD41	TAPS1B41
	HDH25L	4.7	D3844M-P	D4448M-P	CSD47	TAPS1B47
SHAPEONE Tn	HDH25S	4.1	D3338M-P	D3844M-P	CSD41	TAPS1B41
	HDH25L	4.7	D3844M-P	D4448M-P	CSD47	TAPS1B47
iMAX NHSI	HDH25S HDH25L	3.7	D2833M	D3338M-P	CSD37	TAPiMAX37
		4.1	D3338M-P	D3844M-P	CSD41	TAPiMAX41
		4.7	D3844M-P	D4448M-P	CSD47	TAPiMAX47
		5.2	D4448M-P	D4448M-P	CSD52	TAPiMAX52
iMAX NHSIC Regular	HDH25S HDH25L	4.1	D3338M-P	D3844M-P	CSD41	TAPiMAX41
		4.7	D3844M-P	D4448M-P	CSD47	TAPiMAX47
		5.2	D4448M-P	D4448M-P	CSD52	TAPiMAX52
Volution SVB	HDH21S HDH21L	3.3	D2428M	D2833M	CSD33	
		3.7	D2833M	D3338M-P	CSD37	
	HDH25S HDH25L	4.1	D3338M-P	D3844M-P	CSD41	
		4.7	D3844M-P	D4448M-P	CSD47	
		5.2	D4448M-P	D4448M-P	CSD52	
iMAX NHSE	HDH27S HDH27L	3.7	D2833M	D3338M-P	CSD37	TAPiMAX37
		4.1	D3338M-P	D3844M-P	CSD41	TAPiMAX41
		4.7	D3844M-P	D4448M-P	CSD47	TAPiMAX47
		5.2	D4448M-P	D4448M-P	CSD52	TAPiMAX52
SHAPEONE T (abutment included in the pack)	HDH25S	4.1	D3338M-P	D3844M-P	CSD41	TAPS1B41
	HDH25L	4.7	D3844M-P	D4448M-P	CSD47	TAPS1B47
SHAPEONE T (after removing the abutment tighten the implant)	HDH31S	4.1	D3338M-P	D3844M-P	CSD41	TAPS1B41
	HDH31L	4.7	D3844M-P	D4448M-P	CSD47	TAPS1B47

SHAPEONE

Ø 4.1

Sink countersink: up to 1.4mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink and 4.1 tap

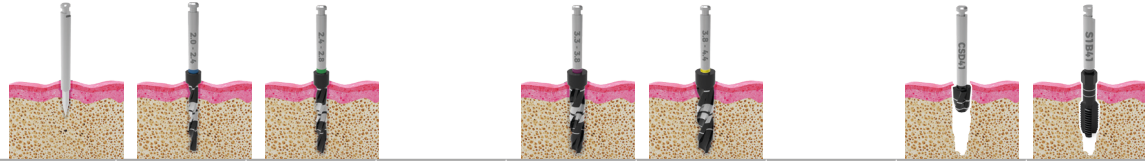

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•		•				
Medium d3/d2	•	•	•		•	•		•	
Compact d1	•	•	•		•	•		•	•

ø 4.7


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.7 countersink and 4.7 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•	•		•			
Medium d3/d2	•	•	•	•		•	•	•	
Compact d1	•	•	•	•		•	•	•	•

ø 3.7


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.7 countersink and 3.7 tap

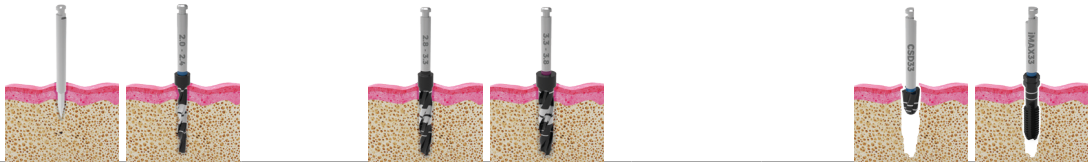

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•		•					
Medium d3/d2	•	•		•	•			•	
Compact d1	•	•		•	•			•	•

ø 4.1


Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink and 4.1 tap

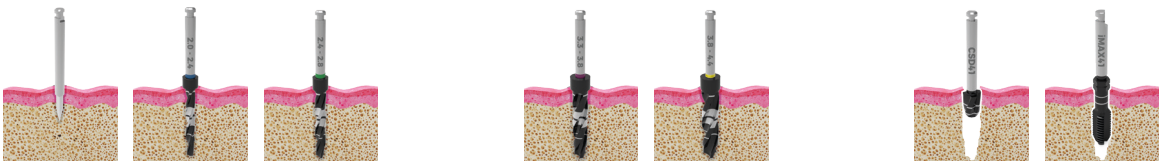

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•		•				
Medium d3/d2	•	•	•		•	•		•	
Compact d1	•	•	•		•	•		•	•

ø 4.7


Sink countersink: up to 1.4mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.7 countersink and 4.7 tap



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•	•		•			
Medium d3/d2	•	•	•	•		•	•	•	
Compact d1	•	•	•	•		•	•	•	•

ø 5.2

Sink countersink: up to 1.4mm for d3 medium bone/ up to 2.8mm for d2 medium bone and d1 compact bone
Use 5.2 countersink and 5.2 tap

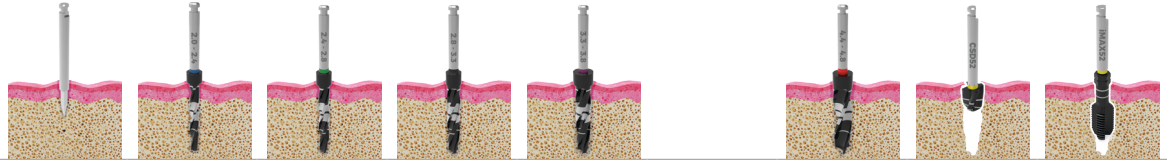


	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8	Step 9
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink	Tap
Soft d4	•	•	•	•	•		•		
Medium d3/d2	•	•	•	•	•		•	•	
Compact d1	•	•	•	•	•		•	•	•

VOLUTION

ø 3.3


Sink countersink: up to 1.4mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.3 countersink



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•		•					
Medium d3/d2	•		•	•				•
Compact d1	•		•	•				•

Ø 3.7

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 3.7 countersink

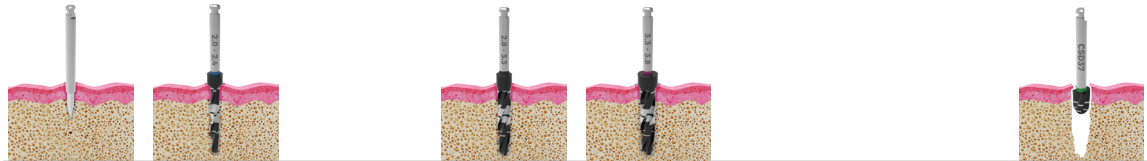

	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•	•		•				
Medium d3/d2	•	•		•	•			•
Compact d1	•	•		•	•			•

Ø 4.1

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.1 countersink



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•	•	•		•			
Medium d3/d2	•	•	•		•	•		•
Compact d1	•	•	•		•	•		•

Ø 4.7

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 4.7 countersink



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•	•	•	•		•		
Medium d3/d2	•	•	•	•		•	•	•
Compact d1	•	•	•	•		•	•	•

Ø 5.2

Sink countersink: up to 1.4 mm for d3 medium bone/ up to 2.8 mm for d2 medium bone and d1 compact bone
Use 5.2 countersink



	Step 1	Step 2	Step 3	Step 4	Step 5	Step 6	Step 7	Step 8
Bone	Lance drill	Drill 2.0 2.4	Drill 2.4 2.8	Drill 2.8 3.3	Drill 3.3 3.8	Drill 3.8 4.4	Drill 4.4 4.8	Countersink
Soft d4	•	•	•	•		•		
Medium d3/d2	•	•	•	•		•	•	•
Compact d1	•	•	•	•		•	•	•

GUIDED SURGERY




GUIDED SURGERY KIT

€
2.625

<i>cod</i>	<i>descrizione</i>
BP	bone profile chirurgia guidata
GD202406	drill ø 2.0/2.4 x 6 mm
GD202408	drill ø 2.0/2.4 x 8 mm
GD202410	drill ø 2.0/2.4 x 10 mm
GD202411	drill ø 2.0/2.4 x 11 mm
GD202413	drill ø 2.0/2.4 x 13 mm
GD202416	drill ø 2.0/2.4 x 16 mm
GD242806	drill ø 2.4/2.8 x 6 mm
GD242808	drill ø 2.4/2.8 x 8 mm
GD242810	drill ø 2.4/2.8 x 10 mm
GD242811	drill ø 2.4/2.8 x 11,5 mm
GD242813	drill ø 2.4/2.8 x 13 mm
GD242816	drill ø 2.4/2.8 x 16 mm
GD283306	drill ø 2.8/3.3 x 6 mm
GD283308	drill ø 2.8/3.3 x 8 mm
GD283310	drill ø 2.8/3.3 x 10 mm
GD283311	drill ø 2.8/3.3 x 11,5 mm
GD283313	drill ø 2.8/3.3 x 13 mm
GD283316	drill ø 2.8/3.3 x 16 mm
GD333806	drill ø 3.3/3.8 x 6 mm
GD333808	drill ø 3.3/3.8 x 8 mm
GD333810	drill ø 3.3/3.8 x 10 mm
GD333811	drill ø 3.3/3.8 x 11,5 mm
GD333813	drill ø 3.3/3.8 x 13 mm
GD333816	drill ø 3.3/3.8 x 16 mm
GD384406	drill ø 3.8/4.4 x 6 mm
GD384408	drill ø 3.8/4.4 x 8 mm
GD384410	drill ø 3.8/4.4 x 10 mm
GD384411	drill ø 3.8/4.4 x 11,5 mm
GD384413	drill ø 3.8/4.4 x 13 mm
GD384416	drill ø 3.8/4.4 x 16 mm
GDCSD33	countersink ø 3.3
GDCSD37	countersink ø 3.7
GDCSD41	countersink ø 4.1
GDCSD47	countersink ø 4.7
GDTAPS1B37	S1B taps ø 3.7
GDTAPS1B41	S1B taps ø 4.1
GDTAPS1B47	S1B taps ø 4.7
GDTAPIMAX33	iMAX taps ø 3.3
GDTAPIMAX37	iMAX taps ø 3.7
GDTAPIMAX41	iMAX taps ø 4.1
GDTAPIMAX47	iMAX taps ø 4.7
PING15 (3 psc)	pin per guidata ø 1.5
HDH25S	short internal hexagon connector 2.5
MDL	hexagonal screwdriver 1.25 h. 29
FR15L	drill D15
CS	guided surgery mucotome
TRT	abutment extractor
GD444806	drill ø 4.4/4.8 x 6 mm
GD444808	drill ø 4.4/4.8 x 8 mm
TWA4	ratchet wrench

Add the mounters (p. 75) according to the implant connection

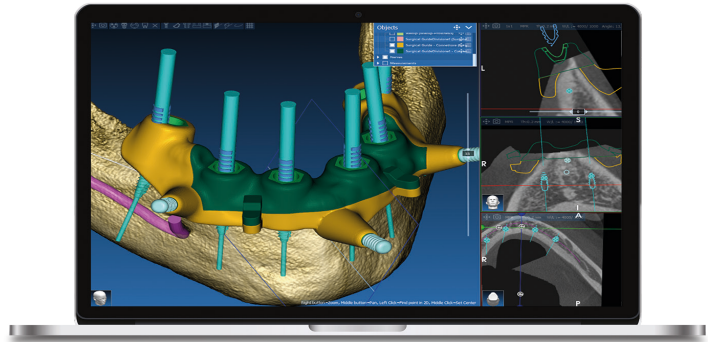

IMPLANT LIBRARIES FOR GUIDED SURGERY

iRES offers to its customers a free kit of implant libraries for the planning of guided surgery procedures. All iRES implants are included in IESS Guide, the diagnostic and guided surgery software proposed by IESS Group based on Real Guide, which accurately reprocesses the patient's anatomical data and facilitates the definition of the ideal treatment plan.

Comprehensive and versatile, thanks to the extensive implant library, the implant placement can be planned taking into account not only the anatomical characteristics of the site but also the prosthetic aspects, in order to achieve functional and aesthetic rehabilitation.

iRES implant libraries are available on the website <https://it.ires.dental/media-kit/> for the following software:

IESS Guide (RealGuide)

Exocad

BlueSky Bio

3Shape Implant Studio

Upon request, libraries can also be created for other software.

PIN Ø 1,5

Material: Ti-6Al-4V



code	€
PING15	26

DRILLS Ø 1.5

Material: Surgical steel



code	€
FR15L	70

DRILLS Ø 2,0/2,4*Material: Surgical steel*

h.	cod	€
6	GD202406	68
8	GD202408	68
10	GD202410	68
11	GD202411	68
13	GD202413	68
16	GD202416	68

**DRILLS Ø 2.4/2.8***Material: Surgical steel*

h.	cod	€
6	GD242806	68
8	GD242808	68
10	GD242810	68
11	GD242811	68
13	GD242813	68
16	GD242816	68

**DRILLS Ø 2.8/3.3***Material: Surgical steel*

h.	cod	€
6	GD283306	68
8	GD283308	68
10	GD283310	68
11	GD283311	68
13	GD283313	68
16	GD283316	68

**DRILLS Ø 3.3/3.8***Material: Surgical steel*

h.	cod	€
6	GD333806	68
8	GD333808	68
10	GD333810	68
11	GD333811	68
13	GD333813	68
16	GD333816	68

**DRILLS Ø 3.8/4.4***Material: Surgical steel*

h.	cod	€
6	GD384406	68
8	GD384408	68
10	GD384410	68
11	GD384411	68
13	GD384413	68
16	GD384416	68

**DRILLS Ø 4.4/4.8***Material: Surgical steel*

h.	cod	€
6	GD444806	68
8	GD444808	68

**COUNTERSINKS***Material: Surgical steel*

∅	cod	€
3.3	GDCSD33	89



∅	cod	€
3.7	GDCSD37	89



∅	cod	€
4.1	GDCSD41	89



∅	cod	€
4.7	GDCSD47	89

IMAX TAPS*Material: Surgical steel*

∅	code	€
3.3	GDTAPIMAX33	89



∅	code	€
3.7	GDTAPIMAX37	89



∅	code	€
4.1	GDTAPIMAX41	89



∅	code	€
4.7	GDTAPIMAX47	89

SURGICAL TAP S1B

Material: Surgical steel



∅	code	€
3.7	GDTAPS1B37	89

∅	code	€
4.1	GDTAPS1B41	89

∅	code	€
4.7	GDTAPS1B47	89

BONE PROFILE

Material: Surgical steel



code	€
BP	68

MUCOTOME

Material: Surgical steel



code	€
CS	68

MOUNTER

Material: Ti-6Al-4V • Screw included: S1BRS1



code	€
BL S1B1GSM	58

code	€
NBL S1BN1GSM	58

code	€
NHSIC NARROW NHSICN1GSM	58

Internal hex 2.5

Internal hex 2.1

Conometric connection 2.1



code	€
EH S1EH1GSM	58

code	€
EH 3.3 S1EHN1GSM	58

code	€
STRAIGHT IMAX MUA NHSMGSM	58

External hex 2.7
Screw included: S1EHR1

External hex 2.4
Screw included: S1EHR1

Screw included: NHSMR1

Material: Ti-6Al-4V

SLEEVE



code	€
BPG15	15

code	€
BG001	15

code	€
BG002	15

Per pin
Material: Ti-6Al-4V

∅ 6.2
Material: PEEK

Material: Ti-6Al-4V

DRILL SEQUENCE

IMPLANT Ø 3.3

		heights implant (mm)					
		6	8	10	11.5	13	16
D1 D2-D3 D4	mucotome CS	•	•	•	•	•	•
	bone profile BP	•	•	•	•	•	•
	drill ø 2.0/2.4 L.6	•	•	•	•	•	•
	drill ø 2.0/2.4 L.8		•	•	•	•	•
	drill ø 2.0/2.4 L.10			•	•	•	•
	drill ø 2.0/2.4 L.11.5				•	•	•
	drill ø 2.0/2.4 L.13					•	•
	drill ø 2.0/2.4 L.16						•
	drill ø 2.4/2.8 L.6	•					
	drill ø 2.4/2.8 L.8		•	•	•	•	•
	drill ø 2.4/2.8 L.10			•			
	drill ø 2.4/2.8 L.11.5				•		
	drill ø 2.4/2.8 L.13					•	•
	drill ø 2.4/2.8 L.16						•
	countersink ø 3.3	•	•	•	•	•	•
	taps ø 3.3	•	•	•	•	•	•

IMPLANT Ø 3.7

		heights implant (mm)					
		6	8	10	11.5	13	16
D1 D2-D3 D4	mucotome CS	•	•	•	•	•	•
	bone profile BP	•	•	•	•	•	•
	drill ø 2.0/2.4 L.6	•	•	•	•	•	•
	drill ø 2.0/2.4 L.8		•	•	•	•	•
	drill ø 2.0/2.4 L.10			•	•	•	•
	drill ø 2.0/2.4 L.11.5				•	•	•
	drill ø 2.0/2.4 L.13					•	•
	drill ø 2.0/2.4 L.16						•
	drill ø 2.4/2.8 L.6	•					
	drill ø 2.4/2.8 L.8		•	•	•	•	•
	drill ø 2.4/2.8 L.10			•			
	drill ø 2.4/2.8 L.11.5				•		
	drill ø 2.4/2.8 L.13					•	•
	drill ø 2.4/2.8 L.16						•
	drill ø 2.8/3.3 L.6	•					
	drill ø 2.8/3.3 L.8		•	•	•	•	•
	drill ø 2.8/3.3 L.10			•			
	drill ø 2.8/3.3 L.11.5				•		
drill ø 2.8/3.3 L.13					•	•	
drill ø 2.8/3.3 L.16						•	
countersink ø 3.7	•	•	•	•	•	•	
taps ø 3.7	•	•	•	•	•	•	





IMPLANT Ø 4.1

	heights implant (mm)					
	6	8	10	11.5	13	16
mucotome CS	•	•	•	•	•	•
bone profile BP	•	•	•	•	•	•
drill ø 2.0/2.4 L.6	•	•	•	•	•	•
drill ø 2.0/2.4 L.8		•	•	•	•	•
drill ø 2.0/2.4 L.10			•	•	•	•
drill ø 2.0/2.4 L.11.5				•	•	•
drill ø 2.0/2.4 L.13					•	•
drill ø 2.0/2.4 L.16						•
drill ø 2.4/2.8 L.6	•					
drill ø 2.4/2.8 L.8		•	•	•	•	•
drill ø 2.4/2.8 L.10			•			
drill ø 2.4/2.8 L.11.5				•		
drill ø 2.4/2.8 L.13					•	•
drill ø 2.4/2.8 L.16						•
drill ø 2.8/3.3 L.6	•					
drill ø 2.8/3.3 L.8		•	•	•	•	•
drill ø 2.8/3.3 L.10			•			
drill ø 2.8/3.3 L.11.5				•		
drill ø 2.8/3.3 L.13					•	•
drill ø 2.8/3.3 L.16						•
drill ø 3.3/3.8 L.6	•					
drill ø 3.3/3.8 L.8		•	•	•	•	•
drill ø 3.3/3.8 L.10			•			
drill ø 3.3/3.8 L.11.5				•		
drill ø 3.3/3.8 L.13					•	•
drill ø 3.3/3.8 L.16						•
countersink ø 4.1	•	•	•	•	•	•
taps ø 4.1	•	•	•	•	•	•


IMPLANT Ø 4.7

	heights implant (mm)					
	6	8	10	11.5	13	16
mucotome CS	•	•	•	•	•	•
bone profile BP	•	•	•	•	•	•
drill ø 2.0/2.4 L.6	•	•	•	•	•	•
drill ø 2.0/2.4 L.8		•	•	•	•	•
drill ø 2.0/2.4 L.10			•	•	•	•
drill ø 2.0/2.4 L.11.5				•	•	•
drill ø 2.0/2.4 L.13					•	•
drill ø 2.0/2.4 L.16						•
drill ø 2.4/2.8 L.6	•					
drill ø 2.4/2.8 L.8		•	•	•	•	•
drill ø 2.4/2.8 L.10			•			
drill ø 2.4/2.8 L.11.5				•		
drill ø 2.4/2.8 L.13					•	•
drill ø 2.4/2.8 L.16						•
drill ø 2.8/3.3 L.6	•					
drill ø 2.8/3.3 L.8		•	•	•	•	•
drill ø 2.8/3.3 L.10			•			
drill ø 2.8/3.3 L.11.5				•		
drill ø 2.8/3.3 L.13					•	•
drill ø 2.8/3.3 L.16						•
drill ø 3.3/3.8 L.6	•					
drill ø 3.3/3.8 L.8		•	•	•	•	•
drill ø 3.3/3.8 L.10			•			
drill ø 3.3/3.8 L.11.5				•		
drill ø 3.3/3.8 L.13					•	•
drill ø 3.3/3.8 L.16						•
drill ø 3.8/4.4 L.6	•					
drill ø 3.8/4.4 L.8		•	•	•	•	•
drill ø 3.8/4.4 L.10			•			
drill ø 3.8/4.4 L.11.5				•		
drill ø 3.8/4.4 L.13					•	•
drill ø 3.8/4.4 L.16						•
countersink ø 4.7	•	•	•	•	•	•
taps ø 4.7	•	•	•	•	•	•


MINIMUM IMPLANTS SIZE ALLOWED FOR POSITION

iRES declines all responsibility in case of failure if the information leaflet are not be respected as regard the implants position in relation to implants site and diameters

UPPER

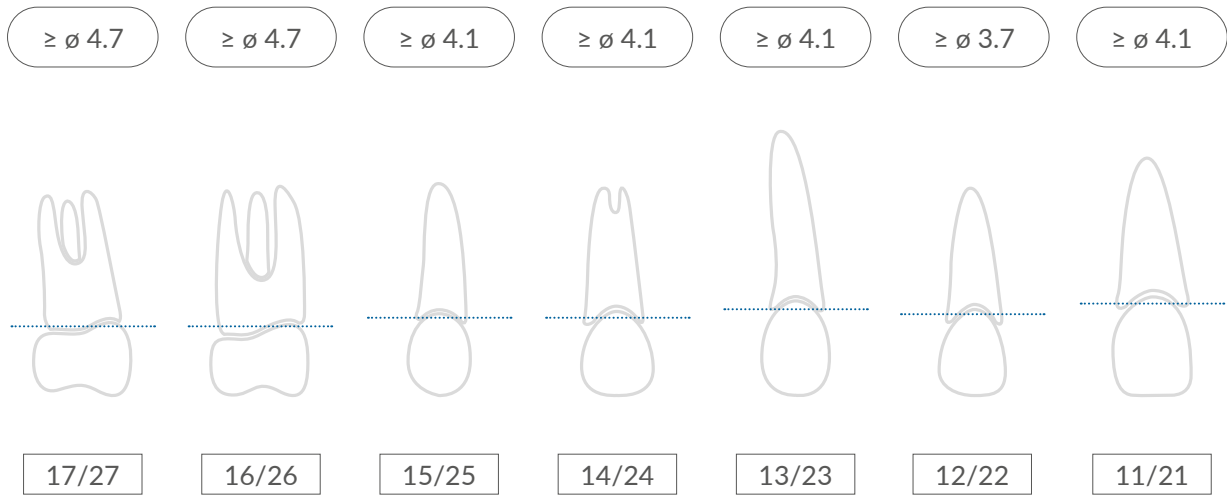

37/47 36/46 35/45 34/44 33/43 32/42 31/41

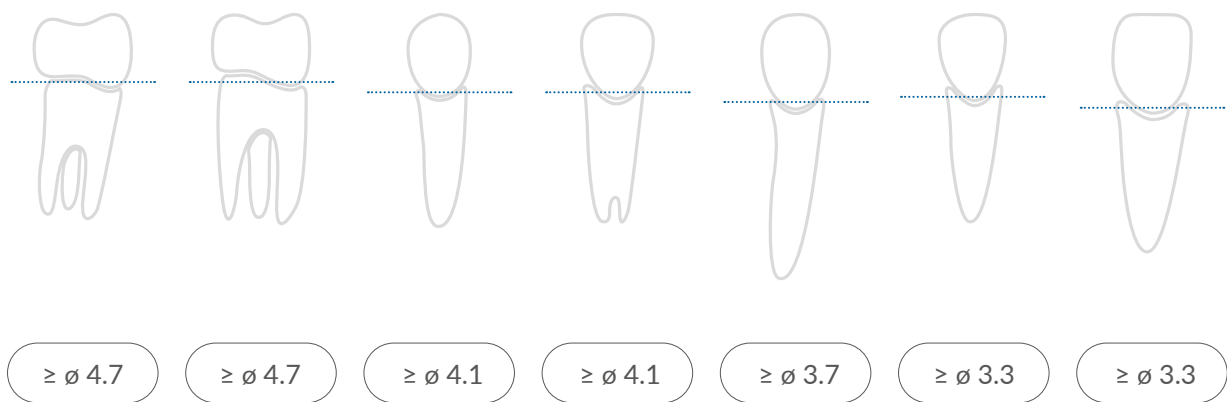

LOWER

INSTRUCTIONS FOR USE I-RES SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY AND SHAPEMINI IMPLANT SYSTEM

PRODUCT CHARACTERISTICS

The **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems, by I-RES SAGL offers the dentist a wide choice of titanium implant configurations that differ in diameter, height and possibility of surgical positioning A) submerged/bone level, B) transmucose/tissue level, and various prosthetic components for the different rehabilitation procedures.

Indications for use

The **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems are indicated for surgical treatment in the upper or lower jaw for the partial or total replacement of teeth in patients who have lost part or all of their teeth. The implant to be used must be chosen by the medical personnel based on the medical history and on the subsequent surgical and prosthetic plan required for each individual patient. The one-piece implants **iMAXMUA**, having the same geometric shape of **iMAX** dental implants, ensure an excellent retention of the prosthesis, thanks to the ability to accommodate the retained screw designed for MUA components with a pitch of 1/72 instead of 1,4 mm as in the classic MUA. The implants are delivered in sterile packs and the operator must pay great attention when positioning it in the oral cavity, so that the implant does not come in contact with elements that could alter the surface, hindering the healing processes, so all manoeuvres must be performed in an environment suitable for surgical activities. The **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant system has a series of dedicated surgical instruments for its implant lines, useful for the non-traumatic preparation of the site that is to receive the implant, and instruments designed for extracting the implant from the blister and transporting it to the mouth for insertion. Each blister containing the implant is provided with a closing screw, useful for sealing the internal part of the implant after it has been inserted in the mandibular or maxillary bone. **SHAPEMINI** implants fix the dentures but can also be used for the replacement of a single tooth.

Contraindications

Do not use **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems in patients who have a scarce amount of bone suitable to guarantee the primary stability of the implant in the first phase of insertion, in patients with poor oral hygiene, smokers, with uncontrolled systemic pathologies and blood disorders. In addition to the normal contraindications for general surgery, the conditions described above can have a negative influence on the partial or total integration of the implant.

Warnings

To use the **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems by I-RES SAGL, the dentist must know the general surgical and prosthetic techniques and the specific techniques for **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI**, following the indications of the surgical protocol and specific training courses. An incorrect choice of implant and surgical technique can be prejudicial to the success of the operation, causing the loss of the implant and of the surrounding bone. No implant must be used that has been used previously, or that has come in contact with the organic elements of third parties. The sterility of the implant is guaranteed by the sealed packaging and by correct storage in controlled dry environments; packages that are not

intact or damaged are prejudicial to the use of the implant. For product traceability it is important to keep the batch number marked on the implant package and on the adhesive labels to be found in the same package. For the same reason it is recommended that the dentist keep as long as possible his patients' medical files, in which he has a record of their medical history, treatment plans, types of operations and prosthetic rehabilitations performed and everything that can be useful for the patient's medical history. The use of non-original I-RES instruments is not advised, as is the failure to follow the indications for inserting the **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems and the respective prosthetic components, because they have been designed to obtain the best result. **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems must be inserted with a maximum torque of 50 Ncm, exceeding this force could be prejudicial to the precision of connection with the subsequent prosthetic part. The **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems include, in their range of implants, very small diameters made not only in pure titanium but also in titanium alloy (such as Ø 3.3 mm, Ø 3.7 mm in the connections internal hexagon and for Ø 2.7 mm for **SHAPEMINI** mini-implants), which must be used as implants only in the front of the mouth and not in diastoric areas where there is great masticatory stress. Especially the mini implants, with a Ø 2.7 mm, may be used only for the anchorage of the prosthesis. Furthermore, the implants with Ø 3.7 mm must not be inserted individually on premolars and molars, but at most should be only linked with bars to distribute the loading force. **SHAPEMINI** mini-implants may be used only in the front part of the mouth for single tooth replacement and not in the rear part of the mouth where masticatory stress are higher, in this sites, they can only be used for dentures anchoring.

THE COMPANY I-RES SAGL DISCLAIMS HERSELF FOR ANY LIABILITY DUE TO THE NON OBSERVANCE OF THE INDICATIONS REPORTED IN THIS INSTRUCTION LEAFLET.

Collateral effects

The known possible collateral effects are the partial or total failure of osseointegration, with consequent loss of the prosthetic function for which the implant system is intended, pain and transient paresthesia, fracture due to excessive load on the implant system, post or prosthesis.

Pre-operative planning

The careful study and assessment of patients who are candidates for implant-prosthetic therapy is of fundamental importance. Physical, instrumental, and radiological examinations and the study of models allow the dentist to make the best diagnosis and consequent therapy. The preparation of the patient for surgical implant therapy and the preparation of the operating room must be given the same care and attention as general surgery; the preparation of the implant site using dedicated drills with controlled revolutions, cooled with saline solution, these are all indispensable conditions for implant therapy.

Surgical complications

Implant surgery operations may lead to some complications that are usually temporary and restricted to the area of operation, such as inflammation, paresthesia, haematoma; there may also be injuries to nerves, to vascular complexes and the membrane of the maxillary sinus. Bone sequestration has rarely occurred.

Materials and packaging












Implant surgery operations may lead to some

complications that are usually temporary and restricted to the area of operation, such as inflammation, paresthesia, haematoma; there may also be injuries to nerves, to vascular complexes and the membrane of the maxillary sinus. Bone sequestration has rarely occurred.

Symbols on the package

The **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implant systems are produced in commercially pure grade 4 titanium - ASTM F67 - and in grade 5 titanium alloy (Ø 3.3 and Ø 3.7 in internal hexagon connections) - ASTM F136. **SHAPE1, iMAX, VOLUTION, iMAXMUA, HANDY and SHAPEMINI** implants are surface treated to improve osseointegration by means of sandblasting followed by double acid-etching. In the market are also available implants with different surface treatments depending on the intended use of the product, as well as implants with a final coating with hyaluronic acid for a better bone tissue healing. The only machined implants are suitable for the patient with periodontitis. The Hybrid implants (presenting a surface half machined and half superficially treated) are specified both for patients with periodontitis and for all those patients where greater care is necessary aimed at reducing or better treating peri-implantitis. Decontamination is performed with cold Argon plasma followed by packaging in a cleanroom, for the final sterilisation phase with gamma or beta rays. The pack containing the implant and the respective cover screw must be opened in a sterile environment in the phases of surgical implant therapy. **I-RES' SAGL** implants are **DISPOSABLE** devices. Their reuse is not desirable from a medical, legal and ethical point of view. The use of not validated sterilization procedures can cause both the infection onset in the patient and impair the product performances. The failure compliance with these instructions implies a different use as provided by the manufacturer and those who make the reuse must take this action on their own responsibility.

SYMBOLS ON THE PACKAGE

	MANUFACTURER I-RES® SAGL Piazzale Roncaa 4 6850 Mendrisio [Switzerland] info@ires.dental www.ires.dental
	(EN) EUROPEAN AUTHORIZED REPRESENTATIVE IESS GROUP SRL Via Madonna della Salute 23 33050 Pozzuolo del Friuli (UD) [Italy]
	CE Mark according to standard MDD93/42/EEC
	Batch number
	Use by
	Sterilized by gamma or beta rays
	Do not reuse
	Do not restitilize
	Follow the instructions given in the illustrative leaflet
	Do not expose to direct sunlight
	Do not expose to rain and keep in an environment free from damp
	Do not use if the packaging is damaged

The I-RES implant-prosthetic system is intended for use in the oral cavity and is provided with useful components to enable the dentist and the dental technician to prosthetically complete the operation begun by the dentist by inserting the implant in the patient. The I-RES implant-prosthetic system completes the line of I-RES dental implants and the respective I-RES instruments.

Product characteristics

Healing screws. The healing screw is a device used by the dentist to keep the oral mucosa pervious in the vicinity of the implant previously inserted. Once the soft tissues have healed, this will allow the dentist to perform the subsequent manoeuvres for prosthetization. The healing screws are made of grade 5 titanium.

Transfer. The transfer in grade 5 titanium is the instrument that allows the transfer from the mouth to a model of the information needed for the prosthetic connection and for making the respective prosthesis. There are two types of transfer: "closed tray and open tray", and they are all composed of two parts (a screw and a repositioner). After being inserted in the implant and secured to it with the screw, the transfer is ready to take the impression in the mouth.

Analog. The analog made of grade 5 titanium has the function of reproducing the internal characteristics of the implant and it must be securely fixed to the transfer. Once joined, the model can be cast.

Straight, angled and millable posts. They are made of grade 5 titanium; they have different shapes depending on the characteristics they have to satisfy, they are used mostly for prosthetic rehabilitations of bridges or crowns. The choice of the device that must be connected to the analog in the first phase is dictated by the clinical and processing decisions, which are at the discretion of the dentist and the dental technician.

Plastic posts. Plastic posts may be divided into two families, one for using directly in the oral cavity, appropriately modified and connected to the post to support temporary prostheses, one for the transformation of plastic posts into metal posts by the dental technician, with processing characteristics that are at the discretion of the dentist and the dental technician.

Gold Bases. These are components made of gold alloy and allow the creation of customized posts using overcasting techniques.

Ball attachments. Ball attachments are made of grade 5 titanium and, once fixed to the implants, they are able to act as an anchorage by means of special attachments to the patient's mobile prosthesis.

Contraindications:

Do not use I-RES products on patients who have allergies to the materials of which the component is made. The use of I-RES components in patients who have metabolic and periodontal diseases or poor oral hygiene may be prejudicial to the success of the

work, as may prosthetic constructions not in line with international standards. The lack of periodic controls, which the patient must undergo with his dentist after prosthetisation, may compromise the life of the implant-prosthetic system.

Warnings:

I-RES prosthetic components are reserved for use by personnel with knowledge of the subject. I-RES points out that alterations to the implant/post connections may be prejudicial to the success of the work, as may the failure to use original components. When using prosthetic components it is important to follow the instructions given by the dentist and the dental technician. When using prosthetic components in the oral cavity it is important to respect the final tightening va-

lue which must be between 20 and 30 Ncm, as better specified in the catalogue.

Collateral effects

Today there are no known collateral effects in the use of I-RES components that can endanger the patient's health.

Prosthetic planning:

The choice of the I-RES components to be used for the case is the specific responsibility of the dentist and of the dental technician, depending on their requirements.

Materials and packaging:

All I-RES prosthetic components are packed in such a way as to be immediately identifiable, once removed from their pack; it is important for the operator to pay great attention in identifying them to avoid changes of position during work. It is useful to make note of the material batch used on the patient's file, for the purpose of traceability. Whether it has been processed or not, before inserting the I-RES prosthetic component in the oral cavity it is of fundamental importance that it be washed and sterilized. Some I-RES components are single-use, so intended for only one patient.

Cleaning | sterilization | storage:

Caution !!! All prosthetic components for dental implants are sold NON-STERILE.

Before use, all prosthetic components must be cleaned, disinfected and sterilized. These processes must also be performed before intraoral use, i.e. before each use for any test phases and in any case before final restoration loading. Repetition of the processes described in this paragraph does not alter the characteristics of these devices. Failure to follow these indications may lead to the onset of infections and complications for the implant and, more generally, for the patient. Important: care must be taken during the subsequent phases in preserving the zone of the connection with the implant (hexagon/octagon/ threading).

a. Cleaning:

In case of automatic cleaning: use an ultrasound bath with a suitable detergent solution. Use neutral detergents only. Follow the manufacturer's instructions concerning concentrations and washing times. Use demineralised water to prevent the formation of stains and marks.

When cleaning manually: use a suitable neutral detergent and follow the manufacturer's user instructions. Brush the products with a soft-bristled brush (non-metal bristles) under running water. Use the brush to apply the detergent to all surfaces. Rinse with distilled water. After rinsing, dry the devices thoroughly and place them inside suitable sterilization bags.

b. Sterilization:

Place in a vacuum autoclave and sterilize as follows: Temperature = 121 - 124°C, with autoclave cycle of at least 20 minutes and drying cycle of 15 minutes.

c. Storage:

After sterilization, the product must remain in the sterilization bags. Only open the bags immediately prior to use. In normal conditions, sterilization bags maintain the sterility of the contents, unless the wrapping is damaged. Therefore, do not use components if the bags in which they were kept are damaged, and re-sterilizes in new bags before using them again. The storage time of products sterilized inside the bags should not exceed that recommended by the manufacturer of the bags.

The product must be stored in a cool dry place, away from direct sunlight, water and heat sources.

ATTENTION:

Some components such as transfers and healing screws are devices that can be reused after.












CLEANING/STERILIZATION/STORAGE (follow the re- spective indications).

DO NOT REUSE a device classified as SINGLE-USE. Although it cannot be seen, it could be mechanically deformed or have been contaminated.

Disposal procedures:

If removed from the oral cavity due to biological or mechanical failure, the prosthetic components must be disposed of as biological waste according to local regulations. More detailed information on the use of the medical device can be found in the specific Surgical Protocol available on the site www.i-res-group.com or in the IRES Shape1 catalogue supplied by the Manufacturer.

Symbols on the package:

-  MANUFACTURER
I-RES® SAGL Piazzale Roncaa 4
6850 Mendrisio [Switzerland]
info@ires.dental
www.ires.dental
-  European Authorized Representative
IESS GROUP SRL Via Madonna della
Salute 23 - 33050 Pozzuolo del Friuli
(UD) [Italy]
-  CE Mark according to standard
MDD93/42/EEC
-  Batch number
-  use before the expiry date
-  Do not reuse
-  Follow the instructions
given in the illustrative leaflet
-  Do not expose to direct sunlight
-  Do not expose to rain and keep in an
environment free from damp
-  Do not use if the packaging is
damaged
-  not sterile

INSTRUCTIONS FOR IRES ROTARY INSTRUMENTS (DRILLS - COUNTERSINKS - TAPS) FOR THE PREPARATION OF THE SITE THAT HAS TO RECEIVE IRES® SHAPE1® IMPLANTS

Product description:

Dental drills, produced by I-RES Sagl, must be used as tools to perforate the bone. The diameters to be used, the lengths and the drilling sequence (number of drills to be used) are the sole choice and decision of the dentist, depending on the surgical protocol that must be followed. The maximum recommended speed is 800 rpm with saline solution applied directly on the drill to assist cooling.

a) The sole purpose of the initial precision drill is to incise the cortical bone in a very precise point where it will later be drilled.

b) The helical drills have laser markings for reference which identify the depth to be reached. Of course, in the use of this type of drill the manual skill and experience of the dental surgeon are extremely important, especially for stopping at the chosen depth.

c) Countersinks are used when it is necessary to widen the initial part of the hole made to adapt the shape that of the neck of the implant to be inserted. The maximum recommended speed is 300 rpm with saline solution applied directly on the drill to assist cooling.

d) Bone taps: in particularly dense bone (type I), before insertion it is advisable to use a bone tap with the same profile as the implant to be inserted. The bone tap has a greater cutting power than the implant, allowing the site to be prepared with reduced trauma. The maximum recommended speed is 30 rpm with saline solution applied directly on the bone tap to

assist cooling.

Materials used:

All I-RES Sagl drills are made of medical grade steel and undergo hardening heat treatment. The maximum recommended number of uses of the devices is 40 times.

Warnings and general precautions:

- It is fundamental to respect the surgical protocol that establishes the diameters, lengths and the sequence of use. The operator is fully responsible for any uses other than those indicated.
- Check that the drills to be used are in good condition, already cleaned and sterilized.
- Check that the drills are in good condition and have not been used more than 40 times.
- Before using them, check that the hand-piece holds the drills perfectly secure and that they rotate in the correct direction.
- Ensure that there is adequate irrigation.
- The application of leverage during drilling could cause breakage of the drill, the hand-piece, or the bone walls on which you are working.

During drilling always exert alternating pressure, using the intermittent drilling technique.

- Always check that the laser marking that indicates diameter and length is clearly visible.
- Any eccentricity or lack of straightness in the drill could result in an oversized hole.

- Wear eye protection, to protect against particles that may be ejected.

CLEANING / STERILIZATION / STORAGE:

The medical devices are supplied NON-STERILE.

Before use, all rotary devices must be cleaned, disinfected and sterilized.

Failure to follow these indications may lead to the onset of infections and complications for the implant and, more generally, for the patient.

a. Cleaning

In case of automatic cleaning: use an ultrasound bath with a suitable detergent solution. Use neutral detergents only. Follow the manufacturer's instructions concerning concentrations and washing times. Use demineralised water to prevent the formation of stains and marks.

When cleaning manually: use a suitable neutral detergent and follow the manufacturer's user instructions. Brush the products with a soft-bristled brush (non-metal bristles) under running water. Use the brush to apply the detergent to all surfaces. Rinse with distilled water. After rinsing, dry the devices thoroughly and place them inside suitable sterilization bags.

b. Sterilization

Place in a vacuum autoclave and sterilize as follows: Temperature = 121 - 124°C, with autoclave cycle of at least 20 minutes and drying cycle of 15 minutes.

c. Storage

After sterilization, the product must remain in the sterilization bags. Only open the bags immediately prior to use. In normal conditions, sterilization bags maintain the sterility of the contents, unless the wrapping is damaged. Therefore, do not use components if the bags in which they were kept are damaged, and re-sterilize in new bags before using them again. The storage time of products sterilized inside the bags should not exceed that recommended by the manufacturer of the bags. The product must be stored in a cool dry place, away from direct sunlight, water and heat sources.

More detailed information on the use of the medical device can be found in the Surgical Protocol. If you do not have a copy, request one from your distributor or directly from the manufacturer.

Symbols on the package:



MANUFACTURER
I-RES® SAGL Piazzale Roncaa 4
6850 Mendrisio [Switzerland]
info@ires.dental
www.ires.dental



European Authorized Representative
IESS GROUP SRL Via Madonna della
Salute 23 - 33050 Pozzuolo del Friuli
(UD) [Italy]



CE Mark according to standard
MDD93/42/EEC



Batch number



Follow the instructions
given in the illustrative leaflet



Do not expose to direct sunlight



Do not expose to rain and keep in an
environment free from damp



Do not use if the packaging is
damaged



Not sterile

INSTRUCTIONS FOR USE OF CLASS I PROSTHETIC COMPONENTS AND SURGICAL INSTRUMENTS

The I-RES implant-prosthetic system is intended for use in the oral cavity and is provided with useful components to enable the dentist and the dental technician to prosthetically complete the operation begun by the dentist by inserting the implant in the patient. The I-RES implant-prosthetic system completes the line of I-RES dental implants and the respective I-RES instruments..

Product characteristic

Transfer

The transfer in gr. 5 titanium is the tool that allows to transfer, from the mouth to a replica model, the information useful for the prosthetic connection and the construction of the respective prosthesis. There are different types of transfers and they are all made up of two parts (a screw and a repositioner). After being inserted into the implant and firmly screwed to it by means of the screw, the transfer is ready to be detected in its position in the oral cavity by means of an impression.

Analog

The analogue is made of gr. 5 titanium and has the function to reproduce the internal characteristics of the implant and must be firmly fixed to the transfer. Once joined, the model can be poured.

Castable abutments

The compatible castable abutments are the most economical and practical prosthetic solution in the implantology field, consisting of a base in castable material such as POM that allow the dental technician to model an implant abutment in wax or resin starting from a pre-built castable base. These abutments will then be completed in their missing anatomical parts by the dental technician and subsequently the entire abutment will be invested and cast in metal alloys. The abutment that will come out of the casting machine will be a replica of the castable base and the modeled portion.

Steel surgical instruments in steel

Ratchet connectors, handpiece connectors, manual screwdrivers, prosthetic screwdrivers, etc., in stainless steel, provide the user with surgical instruments for performing proper dental surgery.

Contraindications:

Do not use I-RES products on patients who have allergies to the materials of which the component is made. The use of I-RES components in patients who have metabolic and periodontal diseases or poor oral hygiene may be prejudicial to the success of the work, as may prosthetic constructions not in line with international standards. The lack of periodic controls, which the patient must undergo with his dentist after prosthesis, may compromise the life of the implant-prosthetic system.

Warnings:

I-RES prosthetic components are reserved for use by personnel with knowledge of the subject. I-RES points out that alterations to the implant/post connections may be prejudicial to the success of the work, as may the failure to use original components. When using prosthetic components it is important to follow the instructions given by the dentist and the dental technician. When using prosthetic components in the oral cavity it is important to respect the final tightening value which must be between 20 and 30 Ncm, as better specified in the catalogue.

Collateral effects

Today there are no known collateral effects in the use of I-RES components that can endanger the patient's health.

Prosthetic planning:

The choice of the I-RES components and surgical instruments to be used for the case is the specific responsibility of the dentist and of the dental technician, depending on their requirements.

Materials and packaging:

All I-RES prosthetic components and surgical instruments are packed in such a way as to be immediately identifiable; once removed from their pack, it is important for the operator to pay great attention in identifying them to avoid changes of position during work. It is useful to make note of the material batch used on the patient's file, for the purpose of traceability.

Whether it has been processed or not, before inserting the I-RES prosthetic component in the oral cavity it is of fundamental importance that it be washed and sterilized. Some I-RES components are single-use, so intended for only one patient.

CLEANING | STERILIZATION | STORAGE:

Caution !!! All prosthetic components for dental implants are sold **NON-STERILE**.

Before use, all prosthetic components must be cleaned, disinfected and sterilized. These processes must also be performed before intraoral use, i.e. before each use for any test phases and in any case before final restoration/loading. Repetition of the processes described in this paragraph does not alter the characteristics of these devices. Failure to follow these indications may lead to the onset of infections and complications for the implant and, more generally, for the patient.

Important care must be taken during the subsequent phases in preserving the zone of the connection with the implant (hexagon/octagon/ threading).

a. Cleaning:

In case of automatic cleaning: use an ultrasound bath with a suitable detergent solution. Use neutral detergent only. Follow the manufacturer's instructions concerning concentrations and washing times. Use demineralised water to prevent the formation of stains and marks.

When cleaning manually: use a suitable neutral detergent and follow the manufacturer's user instructions. Brush the products with a soft-bristled brush (non-metal bristles) under running water. Use the brush to apply the detergent to all surfaces. Rinse with distilled water. After rinsing, dry the devices thoroughly and place them inside suitable sterilization bags.

b. Sterilization:

Place in a vacuum autoclave and sterilize as follows: Temperature = 121 - 124°C, with autoclave cycle of at least 20 minutes and drying cycle of 15 minutes.

c. Storage:

After sterilization, the product must remain in the sterilization bags. Only open the bags immediately prior to use. In normal conditions, sterilization bags maintain the sterility of the contents, unless the wrapping is damaged.

Therefore, do not use components if the bags in which

they were kept are damaged, and resterilized in new bags before using them again. The storage time of products sterilized inside the bags should not exceed that recommended by the manufacturer of the bags.

The product must be stored in a cool dry place, away from direct sunlight, water and heat sources.

ATTENTION:

Some components, such as transfer and surgical instruments, are devices that can be reused after prior follow the respective indications reported in CLEANING/STERILIZATION/STORAGE.












DO NOT REUSE a device classified as SINGLE-USE.


Although it cannot be seen, it could be mechanically deformed or have been contaminated.

Disposal procedures:

If removed from the oral cavity due to biological or mechanical failure, the prosthetic components must be disposed of as biological waste according to local regulations. More detailed information on the use of the medical device can be found in the specific Surgical Protocol available on the site www.ires.dental or in the IRES catalogue supplied by the Manufacturer.

SIMBOLS ON THE PACKAGE

-  Manufacturer
I-RES® SAGL
Piazzale Roncaa, 4
6850 Mendrisio [Switzerland]
info@ires.dental
www.ires.dental
-  European Authorized Representative
IESS GROUP SRL Via Madonna della
Salute 23 - 33050 Pozzuolo del Friuli
(UD) [Italy]
-  CE mark under MDR 17/745
-  Batch number
-  Use before the expiry date
-  Do not reuse
-  Follow the instructions given in the illustrative leaflet
-  Do not expose to direct sunlight
-  Do not expose to rain and keep in an environment free from damp
-  Do not use if the packaging is damaged
-  Not sterile

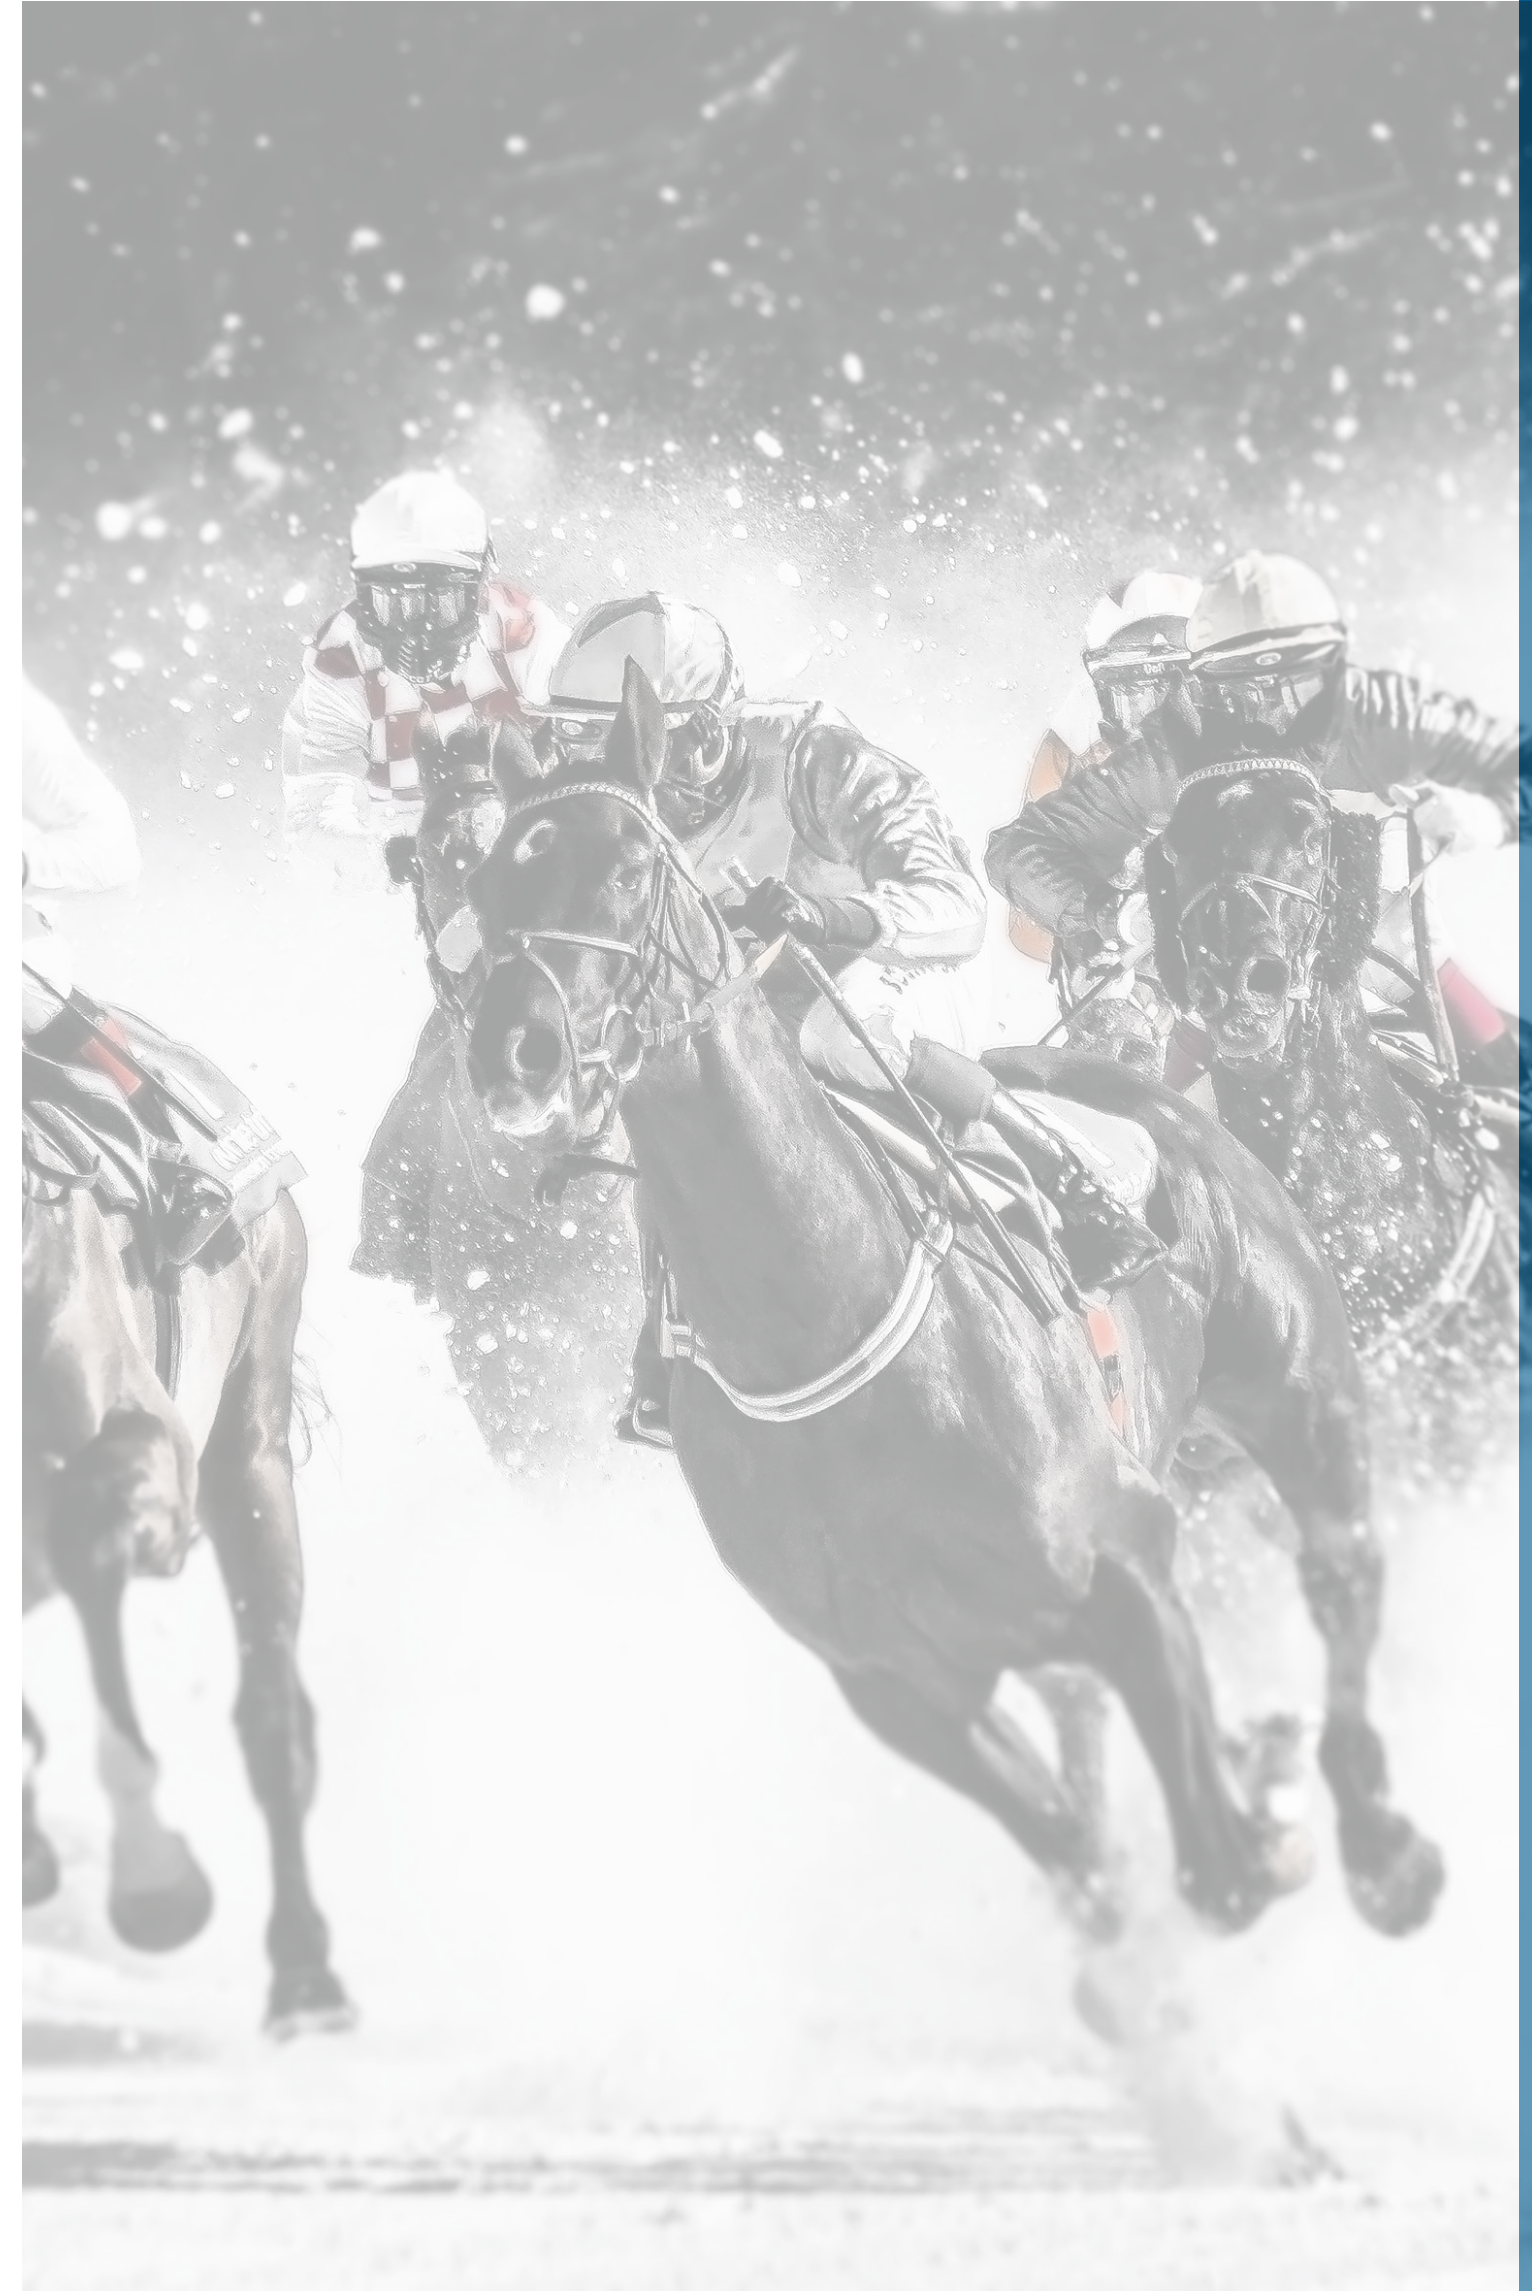

iRES SAGL, a dynamic and flexible company sensitive to the needs of Professionals, offers a complete range of products for oral surgery: **regenerative materials, implant systems, guided surgery, custom prosthesis, Total Implant Care solutions, high-level scientific courses** and programs with Key **Opinion Leaders**.

iRES combines practical experience and **scientific knowledge** to **facilitate procedures** and **improve performance**. This is all possible thanks to a highly professional staff with more than **30 years of experience** in the dental field.

The sales system, based on a **Continuing Education**, involves all Professionals in our scientific programs. **Customer satisfaction is our mission**. High swiss quality meets **advanced technology** to provide an **innovative product concept** and **economically sustainable solutions**.

iRES⁺[®]